

Sorvall
T3/G3
User's Manual



Analyze • Detect • Measure • Control™

Sorvall
T3/G3
User's Manual



T3/G3

Carefully read this manual before operating your instrument.

Information contained in this document is the property of Thermo Fisher Scientific; it may not be duplicated or distributed without the owner's authorization.

The validity of the guarantee is subject to the observation of the instructions and precautions described in this document.

Packing List

<input type="checkbox"/>	75002385	T3	230V 50/60 Hz
<input type="checkbox"/>	75002386	T3	120V 60 Hz
<input type="checkbox"/>	75002396	T3	100V 50/60 Hz
<input type="checkbox"/>	75002387	RT3	230V 50/60 Hz
<input type="checkbox"/>	75002388	RT3	120V 60 Hz
<input type="checkbox"/>	75002397	RT3	100V 50 Hz
<input type="checkbox"/>	75002399	RT3	100V 60 Hz
<input type="checkbox"/>	75003432	G3	230V 50/60 Hz
<input type="checkbox"/>	75003431	G3	120V 60 Hz
<input type="checkbox"/>	75003428	G3	100V 50/60 Hz
<input type="checkbox"/>	75003434	RG3	230V 50/60 Hz
<input type="checkbox"/>	75003433	RG3	120V 60 Hz
<input type="checkbox"/>	75003429	RG3	100V 50 Hz
<input type="checkbox"/>	75003444	RG3	100V 60 Hz

Item number		Quantity	Check
		Centrifuge	<input type="checkbox"/>
11290098	User manual	1	<input type="checkbox"/>
	CE Declaration of compliance	1	<input type="checkbox"/>
	Manual lid opening instructions	1	<input type="checkbox"/>
	Imbalance protection instructions	1	<input type="checkbox"/>
64227001	Mains cord	1	<input type="checkbox"/>
26227005	Toolbox:		
11210935	• Rotor removal tool	1	<input type="checkbox"/>
85241084	• Emergency unlooking tool	1	<input type="checkbox"/>
86000897	• 12 and 13 mm wrench	1	<input type="checkbox"/>

For missing parts call your nearest Thermo representative

WEEE Compliance

Great Britain



WEEE Compliance. This products is required to comply with the European Union's Waste Electrical & Electronic Equipment (WEEE) Directive 2002/96EC. It is marked with the following symbol. Thermo Fisher Scientific has contracted with one or more recycling/disposal companies in each EU Member State, and this products should be disposed of or recycling through them. Further information on Thermo Fisher Scientific's compliance with these Directives, the recyclers in your country, and information on Thermo Fisher Scientific products which may assist the detection of substances subject to the RoHS Directive are available at www.thermo.com/WEEERoHS

Deutschland



WEEE Konformität. Dieses Produkt muss die EU Waste Electrical & Electronic Equipment (WEEE) Richtlinie 2002/96EC erfüllen. Das Produkt ist durch folgendes Symbol gekennzeichnet. Thermo Fisher Scientific hat Vereinbarungen getroffen mit Verwertungs-/Entsorgungsanlagen in allen EU-Mitgliederstaaten und dieses Produkt muss durch diese Firmen widerverwettet oder entsorgt werden. Mehr Informationen über die Einhaltung dieser Anweisungen durch Thermo Fisher Scientific, die Verwerter und Hinweise die Ihnen nützlich sein können, die Thermo Fisher Scientific Produkte zu identifizieren, die unter diese RoHS Anweisung fallen, finden Sie unter www.thermo.com/WEEERoHS

Italia



Conformità WEEE. Questo prodotto deve rispondere alla direttiva dell'Unione Europea 2002/96EC in merito ai Rifiuti degli Apparecchi Elettrici ed Elettronici (WEEE). È marcato col seguente simbolo. Thermo Fisher Scientific ha stipulato contratti con una o diverse società di riciclaggio/smaltimento in ognuno degli Stati Membri Europei. Questo prodotto verrà smaltito o riciclato tramite queste medesime. Ulteriori informazioni sulla conformità di Thermo Fisher Scientific con queste Direttive, l'elenco delle ditte di riciclaggio nel Vostro paese e informazioni sui prodotti Thermo che possono essere utili alla rilevazione di sostanze soggette alla Direttiva RoHS sono disponibili sul sito www.thermo.com/WEEERoHS

Espana



WEEE Conformidad. Este producto requiere cumplir con la Directiva 2002/96EC WEEE (residuos de quipos electricos y electronicos). Este producto esta marcado con el simbolo WEEE, como se describe. En cada Estado Miembro de la Union Europea (EU), Thermo Fisher Scientific ha contratado con diversas companias para disponer y/o reciclar los residuos de equipos electricos y electronicos. Existe informacion adicional acerca de la conformidad de Thermo Fisher Scientific con esta Directiva, incluyendo los nombres de las diversas companias

autorizadas para disponer/recyclar nuestros productos. Adicionalmente suministramos información acerca de los productos de Thermo Fisher Scientific que puedes asistir en la detección de substancias mencionadas en la directiva RoHS, explicado en www.thermo.com/WEEERoHS

France



Conformité WEEE. Ce produit doit être conforme à la directive européenne (2002/96EC) des Déchets d'Équipements Électriques et Électroniques (DEEE). Il est marqué par le symbole suivant. Thermo Fisher Scientific s'est associé avec une ou plusieurs compagnies de recyclage dans chaque état membre de l'union européenne et ce produit devrait être collecté ou recyclé par celles-ci. Davantage d'informations sur la conformité de Thermo Fisher Scientific à ces directives, les recycleurs dans votre pays et les informations sur les produits Thermo Fisher Scientific qui peuvent aider la détection des substances sujettes à la directive RoHS sont disponibles sur www.thermo.com/WEEERoHS

Declaration of compliance	We, Thermo Electron Industries S.A.S., Z.I. d'Aze Bellitourne 53200 CHATEAU-GONTIER, France, declare that the instrument defined here below complies with the following European directives:
Declaration de conformité	Nous, Thermo Electron Industries S.A.S., Z.I. d'Aze Bellitourne 53200 CHATEAU-GONTIER, France, déclarons que le matériel désigné ci-après est conforme aux directives européennes suivantes:
Konformitätserklärung	Wir, Thermo Electron Industries S.A.S. , Z.I. d'Aze Bellitourne 53200, CHATEAU-GONTIER, France, erklären dass das hier beschriebene Gerät sich in Übereinstimmung mit folgenden europäischen Richtlinien befindet:
Declaración de conformidad	Nosotros, Thermo Electron Industries S.A.S., Z.I. d'Aze Bellitourne 53200 CHATEAU-GONTIER, France, declaramos que el instrumento bajo descrito está fabricado según las especificaciones establecidas por las siguientes normas europeas:
Declaração de conformidade	Nós, Thermo Electron Industries S.A.S., Z.I. d'Aze Bellitourne 53200 CHATEAU-GONTIER, France, declaramos que o instrumento aqui apresentado está de acordo com as normas europeias abaixo listadas:
Dichiarazione di conformità	Noi, Thermo Electron Industries S.A.S., Z.I. d'Aze Bellitourne 53200 CHATEAU-GONTIER, France, dichiariamo che lo strumento sotto descritto è conforme alle seguenti Direttive europee:
	<ul style="list-style-type: none"> • Machinery: 98 / 37 / CEE • Low voltage: 72 / 23 / CEE - 93 / 68 CEE • EMC: 89 / 336 CEE - 92 / 31 CEE - 93 / 68 CEE • Safety standard: EN 61010-1 - EN 61010-2-020

Guarantee Terms

Thermo guarantees that this unit is free from defects in materials and workmanship when it leaves the factory, and will replace or repair the unit if it proves defective in normal use or during service for a period of ONE YEAR from the delivery.

This guarantee is invalid if the unit is incorrectly used, poorly serviced or neglected, mis-used or accidentally damaged.

There is no explicit guarantee other than as stated above.

For further information, assistance or service

United States of America

Tel.: +1 888 213 17 90

Tel.: +1 866 984 37 66

Canada or Latin America

Tel.: +1 866 213 17 90

Fax: +1 866 984 37 66

China (Shanghai)

Tel.: +86 21 68 65 45 88

Fax: +86 21 6445 7907, +86 21 6445 7830

India (Mumbai)

Tel.: +91 22 5542 9494

Fax: +91 22 5542 9495

Japan

Tel.: +81 454 53 9220

Fax: +81 454 53 9222

Other Asia-Pacific Countries

Tel.: +852 28 85 46 13

Austria

Tel.: +43 (1) 80 14 00

France

Tel.: +33 1 69 18 77 77

+33 2 28 03 20 00

Belgium

Tel.: +32 24 82 30 30

Germany

Tel.: +49 61 84 90 69 40

Fax: +49 61 03 40 81 012

Finland

Tel.: +35 89 32 91 00

Italy

Tel.: +39 02 95 05 91

Netherlands

Tel.: +31 7 65 71 44 40

Russia/Cis

Tel.: +7 09 52 25 11 15

Spain and Portugal

Tel.: +34 9 32 23 31 54

Switzerland

Tel.: +41 (1) 4 54 12 12

United Kingdom and Ireland

Tel.: +44 87 06 09 92 03

Other Europe, Middle East, or Africa

Tel.: +49 61 8490 6940

Tel.: +33 2 2803 2000

In Other Countries:

Contact your local THERMO products distributor or agent.

E-mail Technical Service Representative for products at:

techsupport.led.asheville@thermo.com

Visit our web site at: www.thermo.com

Contents

Chapter 1	Use and Function.....	1-1
	User Manual.....	1-1
	Warning Symbols.....	1-1
	Description.....	1-1
	Refrigeration and Heating Systems.....	1-2
	Drive System.....	1-3
	Safety Interlock System.....	1-3
	Imbalance Detection System.....	1-3
	Relative Centrifugal Force.....	1-4
Chapter 2	Specifications.....	2-1
	Dimensions and Weight.....	2-1
	Centrifugation Specifications.....	2-1
	Electrical Specifications.....	2-2
Chapter 3	Installation.....	3-1
	Environmental Conditions.....	3-1
	Unpacking.....	3-1
	Positioning.....	3-2
	Mains Supply.....	3-2
	Lid Opening and Rotor Checking.....	3-3
	Manual Lid unlocking Procedure.....	3-3
	Performance and Accessories.....	3-5
	TTH751 Swing-out Rotor - Cat. N°: 11210936.....	3-5
	Angle Rotors.....	3-8
Chapter 4	Instructions for Use.....	4-1
	Controls and Indicators.....	4-1
	Display Screens.....	4-2
	Control Panel Functions.....	4-2
	Control Panel Indicators.....	4-3
	Description of Certain Events with Respect to the Control System.....	4-4
	Preparing the First Run of the Day.....	4-6
	Sample Loading.....	4-6

Chapter 5	Hazards, Precautions and Limitations of Use	5-1
	IEC 1010-2-020.....	5-1
	Cautions.....	5-1
	Speed Control	5-2
	Operational Limitations	5-2
	Aerosol Risks	5-2
Chapter 6	Service and Maintenance	6-1
	Periodic Cleaning.....	6-1
	Contamination Hazards	6-1
	Disinfection	6-2
	Radioactive Decontamination	6-2
	Power Supply Circuit Breaker.....	6-3
	Rotor Removal	6-3
	Trunnion Lubrication.....	6-3
	Chemical Compatibility Table for Rotors, Tubes and Accessories	6-4
Chapter 7	Disposal of Product.....	7-1

Chapter 1 Use and Function

User Manual

The user manual is part of the centrifuge, and contains important information for your safety and for the best use of the equipment

Always keep the manual close to the appliance and in a safe place, so that it is always available. Thermo strongly recommends that all users read this manual carefully.

Warning Symbols

The following symbols are provided to help the operator take advantage of the protection afforded by the equipment and to warn of potential danger.



On the main switch, allows centrifuge to operate. ▲



On the main switch, disconnects the centrifuge from the main power supply. ▲



Only **authorized personnel** can touch the parts close to this symbol and, in any case, only after switching off the main power supply. **Coming in contact with high voltages could cause severe injuries.** ▲



In this manual, this symbol means that you will find important **information for safety**, which if unobserved could result in damage to the appliance and/or harm to the operator. ▲



In this manual, this symbol means that you will find **important information about minimizing** biological risk: if unobserved the result could be harm to the operator. ▲

Description

The T3/G3 centrifuges are designed for laboratory use.

They will separate the components of fluids into layers of varying density by subjecting them to high forces.

Centrifugal force provided by the centrifuge can also be used to drive solvents and low molecular weight solutes through the membrane of a filtering device. Retained macrosolutes will therefore be found above the membrane.

Relative Centrifugal Force (RCF) generated by a rotor is directly proportional to its sedimentation useful radius and to the value of its speed squared.

A control system permits the user, through an extremely intuitive control panel, to set and control the speed, the g-force, the temperature (on the thermostated and refrigerated versions) and the run time, as well as to view different messages and warnings.

Refrigeration and Heating Systems

The T3/G3 Rare ventilated unit. A permanent air circulation reduces the heat level in the bowl.

However the temperature in the bowl can reach 10 °C above the ambient temperature after hours of continuous operation.



The T3/G3 Rare equipped with a powerful refrigeration system that allows samples to be processed at low temperature. The refrigerant, R134a, is free of CFC (Chloro-Fluoro-Carbons) in accordance with the Montreal Protocol directions for preservation of the ozone layer in the atmosphere.

The actual temperature in the bowl is continuously displayed on the front panel of the centrifuge. Under certain conditions (high speed, long duration runs) the sample temperature can be higher than the bowl temperature on the display. In this case, the user may compensate manually after empirical determination of the temperature differential.

Condensation drain on refrigerated units

The lid should remain closed when the refrigeration system is in use to avoid condensation.



The centrifuge has a rubber hose that allows condensation to be drained from the bowl. The drain hose exits at the back of the machine. Near the drain hose you can find the following label:

To remove condensation, please follow this procedure:

- Switch off the centrifuge and disconnect the power.
- Put a small basin under the hose.
- Unplug the hose.

- Drain the centrifuge bowl.
- Insert the plug back into the hose.

Attention Do not remove the plug from the drain hose during centrifugation. ▲

Drive System

A three phase brushless motor drives the rotating equipment. The rotor is contained in a sealed, armor plated centrifugation chamber.

The brushless motor requires no maintenance. A control system ensures the correct drive speed, which is continuously monitored.

Safety Interlock System

The T3/G3 centrifuge series are equipped with an interlock system that assures two basic safety features:

- The run cannot be started if the lid is not correctly closed.
- The centrifuge lid cannot be opened if the rotor is running.

The centrifuge will not operate until the lid is closed and latched in place.

The lid remains latched until the rotor stops spinning. The lid access lamp indicates when the rotor has stopped: consequently the handle on the right hand side of the centrifuge can be used to open the lid.

If a power failure occurs, access to the samples in the centrifuge is possible via a manual lid opening procedure (see appropriate paragraph). For this operation a special tool (supplied with the centrifuge) is required.



Bypass the interlock system only under emergency conditions as the rotor could still be rotating.

Imbalance Detection System

The T3/G3 centrifuge series are equipped with a load imbalance detector.

In case of excessive imbalance, the load imbalance indicator LED is illuminated and the brake is applied immediately. The rotor will be decelerated to rest in few seconds.

As soon as the motor stops, open the centrifuge and redistribute the samples to produce an equal weight on diametrically opposite sides.

If the message persists, despite your efforts to balance the load, call your Thermo Service representative.

Note Imbalance tolerance depends upon the rotor in use. The centrifuge will tolerate 15 gr. of imbalance with the TTH751 rotor equipped with standard buckets. Carefully balance the sample load to avoid actuating the imbalance detection system. If the protection has not been removed from the imbalance detection device during installation, the centrifuge will consider this as an imbalance situation and will not operate.

Relative Centrifugal Force

Relative Centrifugal Force (RCF), at the circumference of a rotor and bucket combination, is directly proportional to the speed (r.p.m.) and radius of the rotor. Therefore, a greater r.p.m. and/or a larger radius produces a greater RCF and improved faster separation of substances. The centrifuge control system carries out and displays the results of all calculations related to speed, radius and RCF.

Note : The value introduced for the radius can be adjusted to allow for position within the tube such as at a boundary. Maximum radii are quoted in the specifications tables. Use of improper radius will adjust the speed setting, automatically applying the wrong RCF.

Chapter 2 Specifications

Dimensions and Weight

	T3	G3	RT3	RG3
Product Dimensions				
Height - lid open (cm / in)	92/ 36.2	134/ 58.8	92/ 36.2	134/ 58.8
Height - lid closed (cm / in)	42/ 16.5	86/ 33.8	42/ 16.5	86/ 33.8
Width (cm / in)	58/ 22.8	58/ 22.8	85/ 33.5	58/ 22.8
Depth (cm / in)	66/ 26.0	66/ 26.0	66/ 26.0	66/ 26.0
Weight unpacked (kg / lb.)	80/176	95/209	106/233	115/253
Packing				
Height (cm / in)	50/ 19.7	99/ 38.9	50/ 19.7	99/ 38.9
Width (cm / in)	70/ 27.6	68/ 26.7	97/ 38.2	68/ 26.7
Depth (cm / in)	67/ 26.4	78/ 30.7	67/ 26.4	78/ 30.7
Weight packed (kg / lb.)	91/201	120/264	116/256	145/319

Centrifugation Specifications

		T3/G3	RT3/RG3
Max capacity	Swing-out	(4x750 mL) 3000 mL	(4x750 mL) 3000 mL
	Fixed Angle	(8x100 mL)	(8x100 mL)
Max density		1200 kg/m ³	1200 kg/m ³
Max load		3.6 kg	3.6 kg
Max speed	Swing-out	4000 rpm	4500 rpm
	Fixed Angle	7800 rpm	8000 rpm
Max RCF	Swing-out	3810 x g	4822 x g
	Fixed Angle	9115 x g	9588 x g
Max noise		< 66 dBA	< 62 dBA

		T3/G3	RT3/RG3
Microprocessor control		yes	yes
Programs (direct recall)		5	5
Speed set/display	Range	500 - 7800	500 - 8000
	Step	10 rpm at less than 1000 rpm	10 rpm at less than 1000 rpm
		100 rpm at above 1000 rpm	100 rpm at above 1000 rpm
Accuracy		± 20 rpm (display)	± 20 rpm (display)
RCF set/display	Range	20 - 9200	20 - 9600
	Step	1 x g	1 x g

	T3/G3	RT3/RG3
Accuracy	± 1 x g	± 1 x g
Timer set/display	30 s - 99 min + continuous	30 s - 99 min + continuous
Temperature set/display	-	-9°C to +40°C -9°C to +60°C
Acceleration rates	5	5
Braking rates	5 + inertial	5 + inertial
Drive system	direct	direct
Brushless induction motor	yes	yes

Electrical specifications

		T3/G3	RT3/RG3
Nominal operating voltage	230V	230 V ±10%	230 V ±10%
	120V	120 V ±10%	120 V ±10%
Power requirements (maximum)		1200 W	1500 W
Heat output (maximum)		3750 BTU / h	4435 BTU / h

Chapter 3 Installation

Environmental Conditions

General conditions accepted for centrifuge transport and storage are:

- Ambient temperature -20°C to +50°C.
- Relative humidity up to 90%.

General conditions accepted for operating the centrifuge safely are:

- Indoor use.
- Temperature: 5 °C to 40 °C.
- Maximum relative humidity of 85%.
- Maximum altitude: 2000 m
- Installation category: II
- Pollution degree: 2

Unpacking

Due to the weight of the machine, all lifting and transporting must be carried out using proper handling equipment (i.e. fork lift trolley) that complies with current regulations, and by people having undergone the necessary training.



Thermo strongly recommends that all operators comply with the local laws and regulations on safety and health in the workplace.

The machine must be supported from underneath. If it has to be transported without its pallet, for example on a staircase, professional handling assistance is required. ▲

- Unpack the centrifuge, carefully removing any possible accessories and the material supplied for ordinary operations and maintenance.
- Check the contents of the package using the packing list provided above.
- Keep the packaging until the centrifuge has been tested and found fully functional.

Positioning

The machine must be installed in a dust and corrosion free room.



Leave a 30 cm / 12 in. space free on each side of and behind the machine for safety reasons, proper ventilation and maximum cooling performances. ▲

Benchtop Units

Place the centrifuge on a bench top, which must be rigid, horizontal and sufficiently strong to support the centrifuge's weight and small vibrations.

Floor standing units

Place the centrifuge on a horizontal floor.

Main Supply

Check mains and frequency: they must correspond to the values shown on the instrument identification label.



For your safety, check that mains wiring is effectively grounded. Thermo declines all responsibility for any damages due to non-grounding of the machine. ▲

Remember that in order to respect the electrical safety standards related to protection against indirect contact, the supply of power to the instrument must be via a power socket fitted with a protection device ensuring automatic cut-off in the case of an insulation fault. A supply fitted with a circuit breaker of the correct rating complies with this requirement.

Lid Opening and Rotor Checking

Ensure that the centrifuge has been switched ON. Pull the handle on the centrifuge right side towards the front of the unit : the lid is automatically unlocked and opens.

In the case of a mains power outage, opening of the lid is prevented by the lid lock safety device. It is recommended to wait for the mains power to be switched back on so that this safety device enables the lid to be unlocked (refer to 3.6 for manual lid opening).



Carefully clean the inside of the centrifugation chamber removing any packing residues.

In fact, due to air turbulence, solid particles accidentally left in the centrifugation chamber create excessive wear of the chamber itself and of the outer rotating equipment surface. ▲

To install the rotor:

- Check that the motor shaft and rotor are clean

- Put the rotor on the motor shaft
- Secure the rotor on the shaft by turning the hexagonal nut counter-clockwise (with the supplied tool)
- Verify that the rotor cannot be removed by trying to pull it (gently) off the shaft.
- In case you are using a swing-out rotor:
- Gently grease the trunnions
- Put the buckets on the trunnions after verifying that the weight of the buckets is identical (the weight is engraved on the bottom of each bucket).

Manual Lid Unlocking Procedure

In the event of mains non-availability or power failure, opening of the lid is prevented by the lid locking safety device. It is recommended that the user waits for the mains to be switched back on so that this safety device enables the lid to be unlocked.

Manual lid unlocking must only be done by someone informed of the possible danger and of the necessary precautions.



Rotating parts are a risk as they could come in contact with the user or be ejected. There is particularly high risk of injury if:

- The user attempts to manually stop the rotor
- Any object falls inside the centrifugation chamber while the rotor is running. ▲

Manual lid unlocking may be necessary under a very limited number of conditions, such as the urgent recovery of critical samples that could be damaged if left in the centrifuge rotor.

In this case the lid can be opened by using the special tool supplied with the centrifuge.



Always set the power switch to the OFF position before performing this manual procedure, even in the case of a mains power outage. ▲


Should the emergency occur due to power failure during centrifugation wait at least 10 minutes for the end of the rotor rotation. In spite of the absence of noise, the rotor could still be rotating when you need to open the lid manually. Upon opening, lift the lid by hand and observe the rotor (be careful in this operation): if it is still rotating, close the lid and wait.



Figure 1. Insert the unlocking tool horizontally into the hole on the right hand side of the instrument.

Figure 2. While pressing up with your finger, to press down with the unlocking tool, pull the lid lever toward you: the lid opens upwards.

The protection sticker must be replaced after it has been pierced (item N° 85241772).

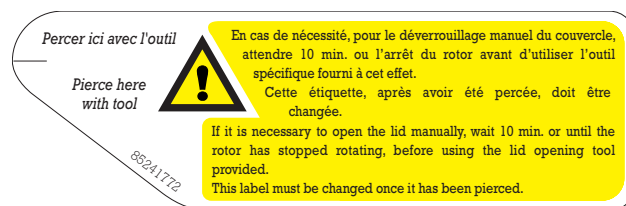

Performance and Accessories

TTH 751 - Swing-out Rotor - Cat. N°: 11210936

- 4500 rpm /4822 x g
- For 4-750 mL bottles
- Up to 148-5 mL tubes
- Up to 16 standard microplates
- Certified sealed accessories are available

11174154	Standard buckets (4)	Inserts: see table
	81005750 750 ml bottles (6)	
	85240471 Cushion (4) - for 750 ml bottles	
11174218	Sealed buckets (4)	Inserts: see table
	81005750 750 ml bottles (6)	
	85240471 Cushion (4) - for 750 ml bottles	
11175372	Bucket - for CORNING 250 ml conical bottles	
11175378	Sealed bucket - for 250 ml conical bottles	
11175370	Bucket - for Nalgene 500 ml flat	
	11175371 Adapters (4) - for 250 ml conical bottle in 11175370	
11210823	Microplate carriers (4)	
	11174207 Rubber cushion - for flexible microtiter plates	
11174223	Sealed microplate carriers (4)	
	11174207 Rubber cushion - for flexible microtiter plates	

Inserts Available for the Following Buckets

- 11174154 Standard buckets (4)
- 11174218 Sealed buckets (4)

Cat. N° (set of 4)	Color of insert or type	Insert Capacity	Rotor Capacity	Max Tube Ø [mm]	Max* tube height [mm]	Tube volume [mL]	Max Radius [mm]	T3/G3		RT3/RG3	
								Max Speed [rpm]	Max RCF [x g]	Max Speed [rpm]	Max RCF [x g]
11174201	Black / light blue	30	120	11.5	40	1.5 / 2	160	4000	2862	4500	3622
11174206	Black / coral	12	48	16.5	40	4 chlamydia vials	184	4000	3291	4500	4166
11174205	Black / beige	9	36	18	40	4 chlamydia vials	184	4000	3291	4500	4166
11174157	Black / grey	37	148	12.5	100	5 ria	172	4000	3077	4500	3894
11174193	Black / grey	decanting	-	12.5	-	5 decant	172	4000	3077	4500	3894
11174158	Black / light blue	30	120	13.5	100	6 rnd/flat	172	4000	3077	4500	3894
11210821	Black	21	108	13.5	107	10 vac	172	4000	3077	4500	3894
11174208	Black / orange	12	48	16.5	125	10 flat	184	4000	3291	4500	4166
11174188	Beige	12	36	18	120	10 flat	172	4000	3077	4500	3894
11174161	Brown	7	28	17.7	134	15 vac	185	4000	3309	4500	4188
11177573	Black	12 unsealed	48	18	122	15 con	188	4000	3363	4500	4256
1175781	Black	10	40	18	122	15 con	188	4000	3363	4500	4256
11174190	Orange	12	48	16.5	125	15	184	4000	3291	4500	4166
11174163	Coral	12	48	22.2	108	20	177	4000	3166	4500	4007
11174186	Dark red	7	28	30	115	25 flat	172	4000	3077	4500	3894
11174164	Dark red	7	28	30	115	50 rnd	182	4000	3256	4500	4120
11174529	Black	7 unsealed	28	30	116	50 con	185	4000	3309	4500	4188
11177572	Black	5	20	30	116	50 con	-	4000	3363	4500	4256
11174199	Light blue	4	16	30	120	50 flat	172	4000	3077	4500	3894
11210560	Light blue	7	28	28		30	177	4000	3166	4500	4007
11174165	Dark blue	4	16	35	120	50 rnd/skirted	185	4000	3309	4500	4188
11174166	Dark green	2	8	45	118	100	185	4000	3309	4500	4188
11174167	Turquoise	1	4	63	134	250 flat flacon con	185	4000	3309	4500	4188
11174192	Navy blue	1	4	80.5	125	450 rnd	185	4000	3309	4500	4188

Inserts Available for the 11175370 Bucket - for Nalgene 500 ml Flat:

Cat. N° (set of 4)	Color of insert or type	Insert Capacity	Rotor Capacity	Max Tube Ø [mm]	Max* tube height [mm]	Tube volume [mL]	Max Radius [mm]	T3/G3		RT3/RG3	
								Max Speed [rpm]	Max RCF [x g]	Max Speed [rpm]	Max RCF [x g]
11175371	-	1	4	-	-	250 con	208	4000	3721	4500	4709

CD 100 - Angle Rotor
Cat. N°: 11210937

Angle rotor

- 8 tubes 100 mL
- 8000 rpm / 9588 x g
- 35° angle

Cat. No.	Insert capacity	Max tube Ø (mm)	Accessory description
64662300	1	16.5 Set of 8	adaptors for 10 mL vac tubes

CD 50c - Angle Rotors
Cat. N°: 11210938


Angle rotor

- 10x50 mL tubes Ø 34mm
- L min/max 97/115mm
- 8000 rpm / 9302 x g
- 35° angle
- conical bottom

Chapter 4 Instructions for Use

Controls and Indicators

All the controls are located on the front panel. The front panel is an intuitive interface: no previous operational knowledge is necessary; every parameter can be set by pressing the cursor key (or rotating the knob) from the minimum to the maximum and viceversa. All parameters can be accessed and changed both during operation and while the machine is at rest.

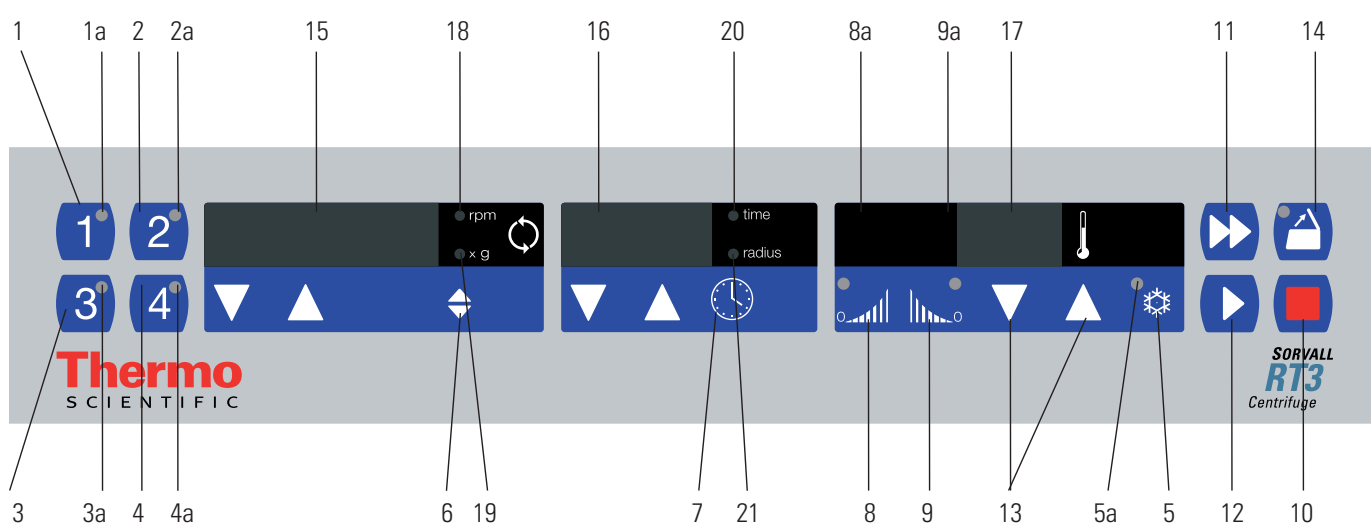

Buttons

- 1 - 4 Program Keys
- 5 Pre Cooling
- 6 Speed/RCF Toggle
- 7 Time/Radius Toggle
- 8 Acceleration rate set
- 9 Deceleration rate set
- 10 Stop Run
- 11 Pulse Run
- 12 Start Run
- 13 Temperature set (R only)

Display Screens

- 15 Display: speed/RCF
- 16 Display: time/radius
- 17 Display: accel./decel. rates/temp. (R mod.)

LED Lights

- 1a Program 1 Indicator
- 2a Program 2 Indicator
- 3a Program 3 Indicator
- 4a Program 4 Indicator
- 5a Program Precooling Indicator
- 8a Acceleration Indicator
- 9a Deceleration Indicator
- 14 Lid Opening allowed Indicator
- 18 Speed Indicator
- 19 RCF Indicator
- 20 Time Indicator
- 21 Radius Input Indicator

Display Screens


Screen	Description
Screen (15)	This screen displays the set speed (rpm) or RCF (x g) for the given program when the centrifuge is at rest, depending on which parameter is selected. During a run, this screen displays actual speed or RCF.
Screen (16)	This screen displays either the set run time or the centrifugal radius when the centrifuge is at rest, depending on which parameter is selected. During a run, this display shows only time remaining (timed runs) or time elapsed (during deceleration, 'hold' runs and 'pulse' runs).
Screen (17)	This screen displays either the acceleration or the deceleration profile selected for the given program. The value of the acceleration profile is displayed either during acceleration or when the acceleration set button (8) is pressed. The value of the deceleration profile is displayed either during deceleration or when the deceleration set button (9) is pressed.
Screen (17) on the R units	This screen displays either the acceleration or the deceleration profile selected for the given program. The value of the acceleration profile is displayed either during acceleration or when the acceleration set button (8) is pressed. The value of the deceleration profile is displayed either during deceleration or when the deceleration set button (9) is pressed. In addition, it shows the temperature in the bowl of the centrifuge. When the centrifuge is at rest, the set bowl temperature is displayed (°C). During a run, the actual bowl temperature is displayed (°C).

Control Panel Functions

Function	Keystroke sequence and description
Start cycle	Press the start button (12).
Stop cycle, immediate	Press the stop button (10).
Pulse	Press the pulse button (11) and hold. The centrifuge will accelerate the rotor to the speed setting of the active program. When the button is released, the rotor will be decelerated to rest.
Set speed	When the LED next to 'RPM' (18) is illuminated, the upper display shows speed values. To increase/decrease the speed values, press on the corresponding up/down arrows.
Set RCF	When the LED next to 'G' (19) is illuminated, the upper display shows RCF values. To increase/decrease the RCF values, press on the corresponding up/down arrows. When using RCF as a control/display value, make sure the correct centrifugal radius is entered into the control system (see below). If an incorrect radius value is in the control system, the RCF value displayed will not be accurate.
Set run time	When the LED next to 'TIME' (20) is illuminated, the middle display shows time values. To increase/decrease the run time values, press on the corresponding up/down arrows.
Set centrifugal radius	When the LED next to 'RADIUS' (21) is illuminated, the middle display shows the value of the centrifugal radius in millimeters. To increase/decrease the centrifugal radius, press on the corresponding up/down arrows. This parameter can only be viewed and set while the centrifuge is at rest. It is essential that this value be correct for the RCF control/display function to be accurate. The correct value of the centrifugal radius depends on the combination of rotor/buckets/adapters being used.

Function	Keystroke sequence and description
Set acceleration profile	When the button (8) is pressed, the lower display (17) shows the number corresponding to the acceleration profile currently registered (1 to 5 : 5 being the fastest). To change the value, press the corresponding up/down arrows.
Set deceleration profile	When the button (9) is pressed, the lower display (17) shows the number corresponding to the deceleration profile currently registered (0= The rotor, from 2000 rpm, will coast to a stop. 1 to 5: 5 being the fastest). To change the value, press the corresponding up/down arrows.
Set temperature (R only)	To increase/decrease the temperature set values, press on the corresponding up/down arrows.
To pre-program the centrifuge	There are five available memory locations for pre-programmed protocols. Each corresponds to one of the five memory buttons (1-5). To enter/save a program into one of the locations, press the memory button corresponding to the desired program position. The corresponding LED (1a-5a) will be illuminated. While the LED is illuminated, enter the desired parameter values. These values are automatically saved in memory.
To lock a program	To lock a program, press and hold the corresponding button for several seconds until the corresponding LED begins to flash. Release the button, and the program is locked. Parameters of the program cannot be changed.
To unlock a program	To unlock a program (when a program is locked, the associated LED flashes), press and hold the corresponding button for several seconds until the associated LED stops flashing. Release the button, and the program is unlocked.
Precooling program	Select the Precooling program pressing button 5, the LED 5a will light on. Only temperature setting is required, Speed and Time are defined by the software according to the rotor in use. Press button 12 to start the precooling program. When the rotor reach the selected temperature, the 5a LED will blink in combination with acoustic signal. Press button 10 to exit. NOTE: The precooling program can not be locked. Use empty rotor without lid.

Control Panel Indicators

Indicator	Description
	When the lid interlock indicator LED (14) is illuminated, the lid interlock is not active. The lid can be opened. The indicator will only be illuminated when the rotor is at rest and it is safe to open the lid. When the lid interlock indicator LED is not illuminated, the lid cannot be opened. The rotor is still in motion. This feature is in accordance with international safety standards.

Description of Certain Events with Respect to the Control System

Start and acceleration phase

When the start button is pressed, the centrifuge will begin to accelerate the rotor. At this point the run timer will start and the middle display will begin to show remaining run time. The upper display will show either actual speed or actual maximum RCF values, whichever is currently selected. The lower display shows the given acceleration profile, and the LED corresponding to the acceleration button is illuminated.

Set error

During acceleration, the centrifuge automatically detects the rotor type and, therefore, its maximum allowed speed. If the operator sets a speed exceeding this, the centrifuge stops acceleration when the maximum allowed speed is reached, ensuring the operator's safety. The display will blink and an audible alarm will invite the operator to correct the speed setting to a proper value.

During the run

During the run, the upper display will show either actual speed or actual maximum RCF values, whichever is currently selected. The middle display will show either remaining time (timed run) or elapsed time ('hold' and 'pulse' runs).

During a run, the middle display will always show time. The user cannot change the display to show the given 'radius' value during a run.

Most set parameters can be changed during a run when the selected program is not locked. Set speed can be changed by selecting speed as the control parameter for the upper display, then by pushing the up or down arrow, or turning the knob. Set run time can be changed by pressing the up or down arrow corresponding to the middle display. Set deceleration profile can be changed by first selecting the deceleration profile (pushing the 'B' button) and then using the up/down arrows, or turning the knob.

Stop and braking (deceleration) phase

When the stop button is pressed (or when the run timer reaches zero), the centrifuge will begin to decelerate the rotor. At this point the run timer will stop and the middle display will begin to show elapsed braking time. The upper display will show either actual speed or actual maximum RCF values, whichever is currently selected. The lower display shows the given deceleration profile, and the LED corresponding to the acceleration button is illuminated.

End of run

At the end of a run, after the rotor has been decelerated to rest, the centrifuge will produce an audible 'beep' and the middle display will show the word 'End'. Pressing any button or opening the lid will bring the displays back to their normal 'at rest' configuration (display of set parameters).

Error Codes

Error code	Origin	State of the centrifuge	User's action
01	Incorrect speed measurement	The rotor will brake to a stop. Lid opening is impossible till speed is zero and a 4 minutes- timeout is expired	Wait for rotor to stop. Wait for the 4 minutes timeout. To erase the message, open the lid, turn the power switch off and turn the power switch on
03	Power was interrupted during a run.	At power off the rotor will coast to a stop.	Press any keyboard button to erase this message. Note: if Error 01 has been detected and not cleared, as above described, the alarm reset is possible only after a safety time of 30 minutes
04	Speed > 0 RPM at power ON	The rotor will coast to a stop.	Wait for rotor to stop. Press any keyboard button to erase this message.
CLOSE Lid	Lid open at start	The centrifuge doesn't start if the lid isn't properly closed	Press any keyboard button to erase this message. Close the lid and press "START"
06	Lid open in running mode	The rotor will brake to a stop.	Wait for the centrifuge to stop. Press any keyboard button to erase this message.
IMBAL	Imbalance.	The rotor will brake to a stop.	Wait for the centrifuge to stop. Press any keyboard button to erase this message. Verify that a balanced load is installed. Inspect the rotor and rearrange the tubes, or add additional tubes with fluid to balance the rotor.
08	Motor Over-temperature OR Lid lock error	The rotor will brake to a stop.	Wait for the centrifuge to stop. Press any keyboard button to erase this message. Wait for motor cooling down.
09	Chamber Over-Temperature The unit displays this code if the measured temperature exceeds 50°C, at any time during the run.	The rotor will brake to a stop. Refrigeration Failure (Refrigerated only)	Wait for the centrifuge to stop. Press any keyboard button to erase this message. Verify the operating condition.
11	Electronic failure	All controls are disabled	To erase the message turn the power switch off and turn the power switch on

Note All error indications can be cleared by turn the power switch off and turn the power switch on.

If error code reappears and the cause of the problem can't be removed contact your local Thermo Service representative ▲

Preparing the First Run of the Day

Before installation, the rotor should be thoroughly inspected for evidence of corrosion or other damage and for cleanliness.

Chemical and stress corrosion of metallic parts will eventually lead to disruption of the rotor with potential severe damage to the centrifuge.

Particles stuck inside the pockets can cause breakage of tubes and lead to major imbalance and / or loss of sample and contamination.

The central hole of the rotor and the drive spindle should also be clean and undamaged. These parts should be wiped clean before each use.

The centrifuge also should be observed to verify proper appearance of screws, lid hooks, latches and for evidence of corrosion.



In case of problems contact your Thermo Service representative, because any deviation from the above mentioned advice may have serious consequences for the safety of the appliance and of the operators. ▲



Normal use of the centrifuge could require the manipulation of biohazards. Users and service personnel must have specific training for each substance they use, according to the “Laboratory Biosafety Manual” from the World Health Organization. ▲

Sample Loading

The contents of each rotor pocket including sample, tube, cap and adapter (where used) must be of the same weight as the one diametrically opposite.




Imbalance of the rotor may cause major damage to the rotor and centrifuge. ▲


Do not attempt to introduce liquids into rotor pockets or into tubes already in the pockets.

Distribute the load correctly. Loads should be inserted two by two, samples of equal weight, at 180 degrees from the rotation axis and at equal distance (radius) from the center of rotation (see pictures).

When using fixed angle rotor, weight deviation between the tubes must not exceed ± 5 grams.

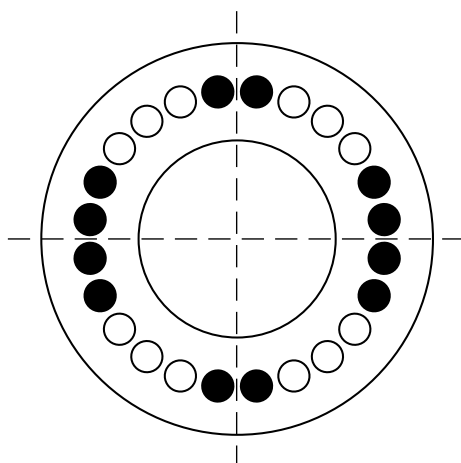


Correct

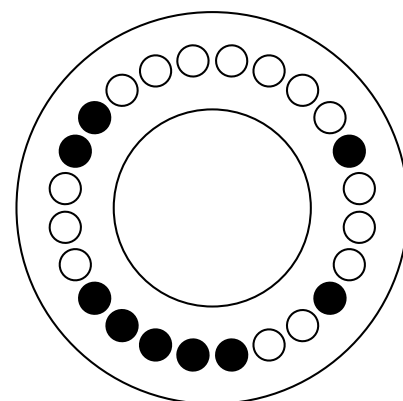


! Incorrect

When using a swing-out rotor, the samples are placed in plastic inserts. The load must be statically and dynamically balanced:

- Static balancing consists of balancing the weight of the 2 inserts which are in opposite locations in the rotor (± 15 to 20 grams).
- Dynamic balancing consists of placing the tubes in each insert symmetrically according to the axis of the trunnions.

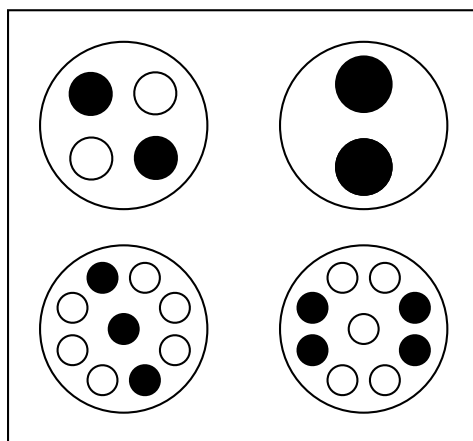

Dynamic Balancing : Correct

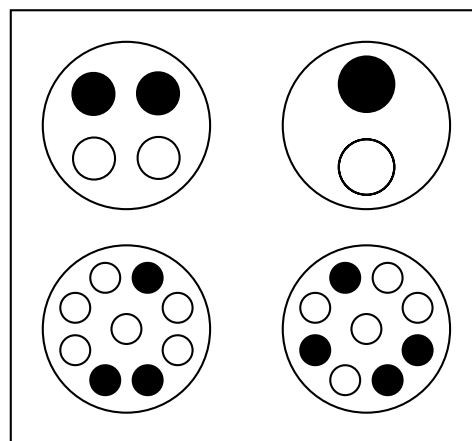

! Incorrect

If less than the maximum complement of samples is loaded, the tubes must be placed in opposite pockets.

An odd number of tubes requires an additional blank, water-filled tube of identical total weight to balance.

Significant vibrations can damage the accessories, the unit and the samples. Most vibration is caused by incorrect loading of the tubes. For

this reason, the centrifuge is equipped with an imbalance detector.

In case of excessive imbalance, the load imbalance indicator LED is illuminated and the brake is applied immediately. The rotor will be decelerated to rest in few seconds.

As soon as the motor stops, open the centrifuge and redistribute the samples to produce an equal weight on diametrically opposite sides.

Also remember that the pins must be softly lubricated. Inadequate lubrication of the pins may cause incorrect swinging of the buckets resulting in imbalance phenomenon. See chapter 6.6 for details.

If the message persists, despite your efforts to balance the load, call your Thermo Service representative.

Chapter 5 Hazards, Precautions and Limitations of Use

IEC 1010-2-020

This centrifuge conforms to the IEC 1010-2-020 international standard, which specifies particular safety requirements for laboratory centrifuges.

According to the standard warnings, the operator must respect the following precautions:

- Mark a boundary area of 30 cm around the centrifuge.
- No person or hazardous material can stay within this boundary longer than necessary for operational reasons, while the centrifuge is operating.
- An emergency switch for disconnection of the mains, in case of malfunction, has to be available and familiar to all the persons operating the centrifuge. This switch has to be remote from the laboratory centrifuge, preferably outside the room in which the centrifuge is located, or adjacent to the exit from that room.

Cautions



- Moving or shifting the machine during centrifugation is dangerous.
- Using the centrifuge with rotating equipment showing evidence of corrosion and wear marks, manipulating and/or tampering with the electronic and mechanical parts are dangerous operations.
- Never try to bypass the lid lock safety while the rotor is spinning.
- Do not try to open the lid until the display returns to the stand-by mode.
- Only use a correctly grounded power source.
- Use only rotors and accessories designed for use in these centrifuges. ▲

Pay special attention to the following:

- Installation of the unit: proper ventilation, leveling of the centrifuge, rigidity and stability of the support.

- Rotor installation: verify that the rotor is locked in position before use.
- Cleaning of the accessories and of the rotor chamber is particularly necessary when corrosive products are present in the samples (saline, acids, bases).
- Load balancing.

IF ANY DANGEROUS EVENT OCCURS, KEEP YOURSELF FAR AWAY FROM THE INSTRUMENT AND SWITCH OFF THE MAIN POWER SOURCE

Speed Control

A view port located on the lid allows the measurement of the actual speed by a phototachometer.

Once a year, check for correct r.p.m. readout and speed control setting which should be within 100 r.p.m. of the actual.

Operational Limitations

The T3/G3 series of centrifuges and their associated rotors offer a high level of RCF performance. In some cases the maximum possible RCF will exceed the one sustainable by the sample container.

The rotor RCF performance displayed is the maximum available in the rotor pockets. Depending on the sample containers or on other application needs, the maximum RCF which must be used is to be determined by the operator.



The centrifuge is not explosion proof.

Using this centrifuge with explosive samples is entirely at the user's own risk. Do not under any circumstances use the centrifuge in an explosive environment. ▲

Aerosol Risks

Due to the action of the turbulence created in the bowl, a centrifuge is an aerosol generator.

A ventilated centrifuge (like the T3/G3 exhausts, into the room, air which has passed through its bowl.

Thus the risk of the spread of aerosols is significant in a ventilated centrifuge.

In the case of samples presenting a biological or chemical risk, the operator must take suitable precautions to prevent or reduce this risk.




Thermo recommends the use of sealed buckets, which are certified for bio-containment through worldwide recognized testing procedures performed in recognized external laboratories. ▲

Aerosols are produced naturally when using uncapped tubes or bottles. They are also produced when a container deforms or breaks provoking a small or large sample leak.

We draw your attention to the use of tubes in angle rotors. Even if the liquid level does not touch the cap when in a static state, it could do so during centrifugation and leak. You should therefore follow the instructions of the tube supplier concerning the fill level and sealing of the tube.

Once a biological risk is known or suspected, samples should be placed in a sealed container. Should such containers not be available, sealed accessories should be used, such as angle rotors with sealed lids.

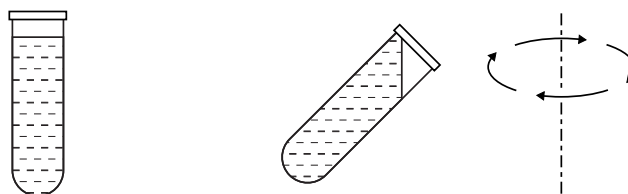

Duration of aerosol presence

When aerosols are created in a centrifuge bowl, they persist in the air for a period of 3-5 minutes after the rotor stops moving. Indeed, the action of opening the lid itself causes the dispersion of aerosols into the environment.



When an elevated risk of aerosols or of breakage is perceived the accessories should be handled using gloves and opened in an environment ensuring the protection of the operator (safety cabinet, glove chamber, wearing a mask ...), even if they are apparently sealed. ▲

Chapter 6 Service and Maintenance



All cleaning operations should be performed with the centrifuge disconnected from the power outlet. ▲

Periodic Cleaning

Daily

No daily cleaning is required, except in the case of accidental tube breakage, or when there is a large amount of spillage in the bowl.

Weekly

Clean the bowl and the accessories with a cotton wool pad dipped in 70% alcohol.

Never use metallic brushes to clean accessories.



- After cleaning the accessories, rinse them in running water, preferably distilled water.
- Dry the rotor with a soft absorbent non-woven cloth or tissue. Drying may be finished off with a warm air jet (e.g. a hair dryer).
- Make sure that the pockets are well dried.
- Ideally, spray with Anti-Corrosion Spray (Cat N° 11175399)
- Store unused buckets upside down on a non-metallic grid to allow free passage of air.

Contamination Hazards

The centrifuge is likely to be used in medical research where hazardous substances, including radioactive chemicals, are frequently found.



ALWAYS USE THE APPROPRIATE DECONTAMINATION PROCEDURES WHEN THE ROTOR IS EXPOSED TO THESE CHEMICALS. ▲

Examples of commonly used techniques are outlined below. The information is given as a guideline only.

It is the responsibility of the owner to use the most suitable procedure. If decontamination procedures require the use of warming (i.e. autoclave) the rotating equipment should always be completely disassembled before being subjected to heat and after external chemical cleaning.

Seals should be decontaminated with the method most suitable for them.

Disinfection

Alcohol (70% ethanol or isopropanol) applied for 10 minutes is ideal for bacteria and viruses.

Autoclave for 20 minutes at 120°C to destroy micro-organisms.

Polypropylene components are autoclaveable.

Rotor lids must be disassembled from rotor bodies. 'O' rings, autoclaved separately, should be replaced when deformed.

Any part which has been subjected to temperatures above 130 °C must be discarded.

Hypochlorite "bleach" used at 0.1% concentration with 10 minutes immersion is effective against bacteria, spores and viruses but, as an oxidizing agent, is corrosive to metal alloys and must be thoroughly rinsed off of metal parts and the parts dried. It should never be used if there is surface damage to the rotor.

Formalin (37% formaldehyde in water) in contact for 10 minutes has a similar effect to chlorine bleaches.

Rotors should be thoroughly rinsed under running water for 5 minutes to remove all traces of formalin then dried completely.



Formaldehyde is toxic. ▲

Gluteraldehyde 2%, sold under many brand names such as Cidex and Glutarex, requires total immersion for 10 minutes to ensure sterility. Thorough rinsing and drying is essential to protect users.



Gluteraldehyde builds up to a toxic level in the fatty tissues of the body. Phenols are very corrosive and should never be used. ▲

Radioactive Decontamination

We recommend that all radioactive contamination be referred to your Radioactivity Safety Officer.

Rotors may be decontaminated by a mixture of equal volumes of:

- Distilled water,
- SDS diluted to 10%,
- Ethanol diluted to 70%.

The rotor should then be rinsed with ethanol followed by distilled water and then dried completely.

Thermo makes no claims as to the effectiveness of proprietary brands of decontaminating solutions.

Power Supply Circuit Breaker

If the main circuit breaker of the centrifuge cuts off the power to the instrument, do not attempt to switch it on before a Thermo Service representative has checked over the unit.

Trunnion Lubrification

This operation is necessary to allow the buckets to swing freely. Clean the trunnions regularly with a dry wipe (as well as the part of the bucket that rotates on the trunnions). Then, put a very small quantity of grease on the curved face of the trunnion. Do not apply too much grease because it will eventually coat the bowl of the centrifuge as centrifugal force pulls the grease from the trunnions.



If the centrifuge is having imbalance problems, try this operation before calling Thermo service. In many cases, imbalance problems arise due to the fact that poorly maintained bucket-trunnion interfaces prevent the buckets from swinging freely. ▲

Chemical Compatibility Table for Rotors, Tubes and Accessories

- | | | |
|---------------------------------|----------------------------------|------------------------|
| S = Satisfactory | AL = Aluminum | BN = Buna N |
| D = Discoloration but OK | CAB = Cellulose acetate butyrate | CN = Cellulose Nitrate |
| P = Pure chemical OK | DL = Delrin | KY = Kynar |
| M = Moderate resistance | NO = Noryl | NY = Nylon |
| U = Unsatisfactory | PA = Polyallomer (= PPCO) | PC = Polycarbonate |
| X = Explosion risk !!! | PE = Polyethylene | PP = Polypropylene |
| O = No information | PPCO = Polypropylene Copolymer | PS = Polysulfone |
| d = Less resistance if T > 50°C | SS = Stainless steel | TF = Teflon |
| t = Unsatisfactory if T > 50°C | TZ = Tefzel | TI = Titanium |
| | VA = Viton A | |

Chemical	Material	AL	BN	CAB	CN	DL	KY	NO	NY	PA	PC	PE	PP	PS	SS	TF	TZ	TI	VA
		PPCO																	
Acetaldehyde		S	U	U	U	O	O	O	O	M	U	M	M	O	S	S	M	S	U
Acetamide		O	O	O	O	O	O	O	O	S	U	S	S	S	O	O	O	O	O
Acetic Acid (5%)		S	M	S	S	M	S	S	S	S	S	D	S	S	S	S	S	M	
Acetic Acid (20 %)		S	O	O	O	O	O	O	O	S	M	S	S	S	O	O	O	O	
Acetic Acid (60%)		S	U	U	U	U	S	S	M	S	U	M	D	S	S	S	S	U	
Acetic Acid (80 %)		S	O	O	O	O	O	O	O	S	U	St	S	M	O	O	O	O	
Acetic Acid (Glacial)		S	U	U	U	U	S	O	O	S	U	M	D	M	S	S	S	U	
Acetic Anhydride		S	O	O	O	O	O	O	O	Sd	U	U	Sd	U	O	O	O	O	
Acetone		S	U	U	U	M	M	O	U	S	U	S	M	U	S	S	M	U	
Acetonitrile		O	O	O	O	O	O	O	O	Mt	U	S	Mt	U	O	O	O	O	
Acetylene		S	O	O	O	O	O	O	O	S	O	S	S	U	O	O	O	O	
Adipic Acid		O	O	O	O	O	O	O	O	S	S	St	S	S	O	O	O	O	
Alanine		S	O	O	O	O	O	O	O	S	S	U	S	U	O	O	O	O	
Allyl Alcohol		O	O	U	O	S	O	O	U	O	S	S	S	O	O	S	S	O	
Aluminum Chloride		O	O	S	S	O	S	O	S	S	S	S	S	O	U	S	S	O	
Aluminum Fluoride		O	O	O	O	O	S	O	S	S	U	S	S	O	O	S	O	O	
Aluminum Hydroxide		S	O	O	O	O	O	O	O	S	Mt	Sd	S	S	O	O	O	O	
Aluminum Nitrate		M	O	O	O	O	O	O	O	S	O	O	S	O	O	O	O	O	
Aluminum Sulphate		S	O	O	O	O	O	O	O	Sd	O	S	Sd	O	O	O	O	O	
Amino Acids		S	O	O	O	O	O	O	O	S	S	S	S	S	O	O	O	O	
Ammonia		S	O	O	O	O	O	O	O	S	U	S	S	Sd	O	O	O	O	
Ammonium Acetate		O	O	O	O	O	O	O	O	S	S	S	S	O	O	S	S	O	
Ammonium Carbonate		S	U	S	S	O	S	O	S	S	U	S	S	S	S	S	S	O	
Ammonium Chloride		M	O	O	O	O	O	O	O	St	O	St	St	O	O	O	O	O	
Ammonium Hydroxide (10%)		O	S	U	O	O	O	O	S	D	U	S	D	S	S	S	S	S	
Ammonium Hydroxide (conc)		O	U	U	O	O	O	O	S	D	U	S	D	O	S	S	S	U	
Ammonium Oxalate		O	O	O	O	O	O	O	O	Sd	S	S	Sd	S	O	O	O	O	
Ammonium Phosphate		U	O	O	O	O	O	O	O	S	M	S	S	O	O	O	O	O	
Ammonium Sulphate		S	S	O	O	U	O	O	S	S	S	S	S	O	S	S	S	O	
Ammonium Sulphide		O	O	O	O	O	S	O	O	S	U	O	S	O	O	S	O	O	
n-Amyl Acetate		S	O	O	O	O	O	O	O	Sd	U	Sd	Sd	U	O	O	O	O	
Amyl Alcohol		S	M	U	O	S	O	O	S	S	S	S	S	O	O	S	S	M	
Amyl Chloride		S	O	O	O	O	O	O	O	U	U	U	U	U	O	O	O	O	
Aniline		S	O	O	O	O	S	O	O	U	O	S	M	O	O	S	S	O	

Chemical	Material	AL	BN	CAB	CN	DL	KY	NO	NY	PA	PC	PE	PP	PS	SS	TF	TZ	TI	VA
		PPCO																	
Aqua Regia		U	U	U	0	U	0	0	0	U	U	U	U	0	0	S	S	S	M
Barium Chloride		U	0	0	0	0	0	0	0	S	0	S	S	0	0	0	0	0	0
Barium Hydroxide		U	0	0	0	0	0	0	0	S	0	S	S	0	0	0	0	0	0
Barium Sulphate		S	0	0	0	0	0	0	0	S	0	St	S	0	0	0	0	0	0
Benzaldehyde		S	0	0	0	0	0	0	0	Sd	Mt	S	Sd	M	0	0	0	0	0
Benzene		S	U	P	0	M	0	0	S	U	U	U	U	U	S	S	S	S	S
Benzoic Acid, Sat		St	0	0	0	0	0	0	0	Sd	Sd	S	Sd	M	0	0	0	0	0
Benzyl Acetate		0	0	0	0	0	0	0	0	Sd	Mt	S	Sd	U	0	0	0	0	0
Benzyl Alcohol		S	U	U	0	M	0	0	U	U	U	U	U	0	0	S	S	S	S
Boric Acid		U	0	0	0	0	0	0	0	S	U	Sd	S	U	0	0	0	0	0
Bromine		U	0	0	0	0	0	0	0	U	Mt	U	U	U	U	0	0	0	0
Bromobenzene		U	0	0	0	0	0	0	0	U	U	U	U	U	U	0	0	0	0
Bromoform		U	0	0	0	0	0	0	0	U	U	U	U	U	U	0	0	0	0
Butadiene		S	0	0	0	0	0	0	0	U	U	U	U	U	0	0	0	0	0
Butane		S	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0
n-Butanol		S	S	U	0	S	0	0	U	0	M	S	S	M	0	S	S	S	S
n-Butyl Acetate		S	0	0	0	0	0	0	0	S	U	S	S	U	0	0	0	0	0
Butylene		S	0	0	0	0	0	0	0	0	0	S	0	0	0	0	0	0	0
Butyl Chloride		0	0	0	0	0	0	0	0	U	U	U	U	U	U	0	0	0	0
Butyric Acid		S	0	0	0	0	0	0	0	U	Mt	U	U	S	0	0	0	0	0
Caesium Acetate		M	0	0	0	0	0	0	0	S	S	S	S	S	0	S	S	0	0
Caesium Bromide		M	0	0	0	0	0	0	0	S	S	S	S	S	0	S	S	0	0
Caesium Chloride		M	0	S	S	0	0	0	0	S	S	S	S	S	S	S	S	S	0
Caesium Formiate		M	0	0	0	0	0	0	0	S	S	S	S	S	0	S	S	0	0
Caesium Iodide		M	0	0	0	0	0	0	0	S	S	S	S	S	0	S	S	0	0
Caesium Sulphate		M	0	0	0	0	0	0	0	S	S	S	S	S	0	S	S	0	0
Caesium Trifluoroacetate		M	0	M	U	0	0	0	0	S	S	S	S	S	M	S	0	0	0
Calcium Carbonate		U	0	0	0	0	0	0	0	S	0	St	S	0	0	0	0	0	0
Calcium Chloride		M	S	S	0	S	0	0	S	S	M	0	D	S	S	S	0	S	S
Calcium Hypochlorite		M	U	0	0	M	S	0	S	S	M	S	S	S	U	S	0	S	S
Calcium Sulphate		M	0	0	0	0	0	0	0	S	0	St	S	0	0	0	0	0	0
Carbazole		0	0	0	0	0	0	0	0	S	U	S	S	U	0	0	0	0	0
Carbon Sulphide		S	0	0	0	0	0	0	0	U	U	U	U	U	0	0	0	0	0
Carbon Tetrachloride		X	U	S	S	M	S	0	S	U	U	U	U	S	M	S	S	S	S
Cedarwood Essence		0	0	0	0	0	0	0	0	U	St	U	U	M	0	0	0	0	0
Chlorine, dry		M	0	0	0	0	0	0	0	St	Sd	St	St	0	0	0	0	0	0
Chlorine, moist		U	0	0	0	0	0	0	0	Mt	Sd	St	Mt	0	0	0	0	0	0
Chloroacetic Acid		U	0	0	0	0	0	0	0	Sd	Mt	S	Sd	U	0	0	0	0	0
p-Chloroacetophenone		0	0	0	0	0	0	0	0	S	U	S	S	U	0	0	0	0	0
Chlorobenzene		0	0	U	U	0	S	0	0	U	U	U	U	0	0	S	0	S	0
Chloroform		X	U	M	S	M	S	0	U	U	U	U	U	U	S	S	M	S	S
Chlorosulphonic		M	0	0	0	0	0	0	0	M	0	M	M	0	0	0	0	0	0
Chromic Acid (5 %)		U	0	0	0	0	0	0	0	S	M	S	S	U	0	0	0	0	0
Chromic Acid (10%)		M	U	U	U	U	S	S	0	S	M	S	S	U	U	S	S	S	S
Chromic Acid (50%)		U	U	U	S	U	S	0	0	D	U	S	S	U	U	S	S	M	S
Cinnamon Essence		0	0	0	0	0	0	0	0	U	St	U	U	M	0	0	0	0	0
Citric Acid (10%)		S	S	S	0	M	S	S	M	S	S	S	S	S	S	S	S	S	S
Copper Nitrate		U	0	0	0	0	0	0	0	S	0	S	S	0	0	0	0	0	0

Chemical	Material	AL	BN	CAB	CN	DL	KY	NO	NY	PA	PC	PE	PP	PS	SS	TF	TZ	TI	VA
		PPCO																	
Copper Sulphate		U	0	0	0	0	0	0	0	S	0	St	S	0	0	0	0	0	0
Croesol		S	0	0	0	0	S	0	U	S	U	S	S	0	0	S	M	S	0
Cyclohexane		S	0	0	0	0	0	0	0	Mt	Sd	Mt	Mt	U	0	0	0	0	0
Cyclohexanol		S	0	U	0	0	0	0	S	S	M	S	S	0	0	S	0	S	0
Cyclohexanone		0	0	0	0	0	0	0	0	Mt	U	U	U	U	U	0	0	0	0
Cyclopentane		0	0	0	0	0	0	0	0	Mt	U	U	U	U	U	0	0	0	0
Decane		0	0	0	0	0	0	0	0	Mt	Mt	Mt	Mt	Sd	0	0	0	0	0
Dextran Sulphate		M	0	0	0	0	0	0	0	S	S	S	S	S	0	S	S	0	0
Diacetone		S	0	U	0	0	0	0	0	S	0	S	S	0	0	S	0	S	0
Diacetone Alcohol		S	0	0	0	0	0	0	0	S	0	S	S	0	0	0	0	0	0
o-Dichlorobenzene		0	0	0	0	0	0	0	0	Mt	U	Mt	Mt	U	0	0	0	0	0
p-Dichlorobenzene		0	0	0	0	0	0	0	0	Mt	U	Mt	Mt	U	0	0	0	0	0
Dichloroethane		0	U	U	U	S	0	S	S	U	U	U	U	0	0	S	S	S	S
Dichlorophenol		0	0	0	0	0	0	0	0	U	U	U	U	U	0	0	0	0	0
Diethylamine		S	0	0	0	0	0	0	0	St	U	U	St	Sd	0	0	0	0	0
Diethyl Benzene		0	0	0	0	0	0	0	0	U	Mt	U	U	U	0	0	0	0	0
Diethylene Glycol		S	S	S	S	S	S	0	U	S	S	S	S	S	0	S	S	S	S
Diethylene Glycol Ethyl Ether		0	0	0	0	0	0	0	0	S	Mt	S	S	M	0	0	0	0	0
Diethyl Ether		S	0	0	0	0	0	0	0	U	U	0	U	0	0	0	0	0	0
Diethyl Ketone		S	0	U	U	M	0	0	U	U	U	M	M	0	0	S	M	S	0
Dimethylacetamide		0	0	0	0	0	0	0	0	S	U	St	S	U	0	0	0	0	0
Dimethylformamide		S	0	0	0	0	0	0	0	S	U	S	S	0	0	S	M	S	0
Dimethylsulphoxide		S	0	0	0	0	0	0	0	S	U	0	S	0	S	S	M	S	0
Dioxane		S	U	U	0	M	S	0	0	M	U	M	M	0	0	S	S	S	U
Diphenyloxide		S	0	0	0	0	0	0	0	U	0	0	U	0	0	0	0	0	0
Dipropylene Glycol		0	0	0	0	0	0	0	0	S	Sd	S	S	S	0	0	0	0	0
Distilled Water		S	S	S	S	S	0	S	S	S	S	S	S	S	S	S	S	S	S
Ethanol (50%)		S	S	S	S	M	S	S	U	S	M	S	S	S	S	S	S	S	S
Ethanol (95%)		S	S	U	U	M	S	S	U	S	U	S	S	S	S	S	S	S	S
Ethyl Acetate		M	U	U	U	M	S	0	U	M	U	S	U	U	0	S	S	S	U
Ethyl Benzene		0	0	0	0	0	0	0	0	Mt	U	St	Mt	U	0	0	0	0	0
Ethyl Benzoate		0	0	0	0	0	0	0	0	Sd	M	S	Sd	U	0	0	0	0	0
Ethyl Butyrate		0	0	0	0	0	0	0	0	St	U	St	St	U	0	0	0	0	0
Ethyl Chloride		S	0	0	0	0	0	0	0	St	U	St	St	U	0	0	0	0	0
Ethylene Chloride		S	0	0	0	0	0	0	0	St	U	St	St	U	0	0	0	0	0
Ethylene Glycol		S	S	S	S	S	S	0	U	S	S	S	S	S	0	S	S	S	S
Ethylene Oxide		0	0	0	0	0	0	0	0	M	Mt	M	M	S	0	0	0	0	0
Ethyl Ether		S	0	U	U	0	0	0	0	M	U	M	M	0	0	S	M	S	0
Ethyl Lactate		0	0	0	0	0	0	0	0	0	S	St	S	S	M	0	0	0	0
Ethyl Malonate		0	0	0	0	0	0	0	0	0	S	Mt	S	S	M	0	0	0	0
Fatty Acids		S	0	0	0	0	0	0	0	Sd	Sd	Sd	Sd	S	0	0	0	0	0
Ferric Chloride		U	S	0	0	M	S	S	S	S	0	S	S	0	U	S	S	S	S
Ferric Nitrate		M	0	0	0	0	0	0	0	S	0	St	S	M	0	0	0	0	0
Ferric Sulphate		S	0	0	0	0	0	0	0	S	0	S	S	0	0	0	0	0	0
Ficoll Paque		M	0	0	0	0	0	0	0	S	S	S	S	S	0	S	S	0	0
Fluorine		S	0	0	0	0	0	0	0	Mt	Sd	St	Mt	U	0	0	0	0	0
Fluorhydric Acid (10%)		U	U	M	M	U	S	0	S	S	M	S	S	S	U	S	S	U	0
Fluorhydric Acid (50%)		U	U	U	U	U	S	0	0	S	U	S	S	M	U	S	S	U	M

Chemical	Material	AL	BN	CAB	CN	DL	KY	NO	NY	PA	PC	PE	PP	PS	SS	TF	TZ	TI	VA
		PPCO																	
Formaldehyde (20%)		S	0	0	0	0	0	0	0	S	Sd	S	S	Sd	0	0	0	0	0
Formaldehyde (40%)		M	M	0	S	0	S	S	S	S	S	S	D	S	S	S	S	S	S
Formaldehyde (50%)		S	0	0	0	0	0	0	0	S	Sd	S	S	Sd	0	0	0	0	0
Formic Acid (100%)		S	M	U	0	U	S	S	U	S	M	S	S	0	U	S	S	S	U
Freon TF		U	0	0	0	0	0	0	0	Sd	Sd	Sd	Sd	Sd	0	0	0	0	0
Fuel Oil		0	0	0	0	0	0	0	0	Sd	Sd	Mt	Sd	Sd	0	0	0	0	0
Glucose		S	0	0	0	0	0	0	0	S	0	S	S	0	0	0	0	0	0
Glutaraldehyde		0	0	0	0	0	0	0	0	Sd	Sd	S	Sd	Sd	0	0	0	0	0
Glycerine		S	0	0	0	0	0	0	0	S	S	S	S	S	0	0	0	0	0
Glycerol		S	0	0	S	0	S	S	0	S	S	S	S	S	S	S	S	S	0
Heptane		S	0	0	0	0	0	0	0	M	0	S	M	0	0	0	0	0	0
Hexane		S	0	0	0	0	0	0	0	S	0	M	S	0	0	0	0	0	0
Hydrazine		0	0	0	0	0	0	0	0	U	U	U	U	U	0	0	0	0	0
Hydrochloric Acid (5%)		U	0	0	0	0	0	0	0	S	S	S	S	S	0	0	0	0	0
Hydrochloric Acid (37 %)		U	0	0	0	0	0	0	0	Sd	U	S	Sd	S	0	0	0	0	0
Hydrochloric Acid (50%)		U	U	U	U	U	S	S	0	M	U	S	M	0	U	S	S	S	M
Hydrochloric Acid (conc.)		U	U	U	0	U	0	0	0	S	U	0	S	0	U	S	S	S	0
Hydrofluoric Acid (10%)		U	U	M	M	U	S	0	S	S	M	S	S	S	U	S	S	U	0
Hydrofluoric Acid (50%)		U	U	U	U	U	S	0	0	S	U	S	S	M	U	S	S	U	M
Hydrogen Peroxide (3%)		S	M	S	S	S	0	S	S	S	S	S	D	S	S	S	S	S	S
Hydrogen Peroxide (100%)		S	U	S	S	U	0	S	0	S	S	S	D	S	S	S	S	U	M
Iodine, Crystals		S	0	0	0	0	0	0	0	Mt	U	U	Mt	U	0	0	0	0	0
Isobutyl Alcohol		0	M	U	0	S	0	0	U	S	S	S	S	0	0	S	S	S	S
Isopropyl Alcohol		U	M	U	U	S	0	S	U	S	M	S	S	M	0	S	S	S	S
Isopropylbenzene		0	0	0	0	0	0	0	0	Mt	U	Mt	Mt	U	0	0	0	0	0
Kerosene		S	0	0	0	0	0	0	0	Sd	S	Mt	Sd	St	0	0	0	0	0
Lactic Acid (20%)		0	S	0	0	0	0	S	0	S	S	S	S	S	S	S	S	S	S
Lactic Acid (100%)		0	S	0	0	0	0	0	0	S	S	S	S	0	S	S	S	S	S
Lead Acetate (aq.)		U	0	0	0	0	0	0	0	S	S	St	S	0	0	0	0	0	0
Lemon Essence		U	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0
Lime, (conc.)		M	0	0	0	0	0	0	0	S	U	S	S	S	0	0	0	0	0
Magnesium Chloride		M	0	0	0	0	0	0	0	S	S	S	S	S	0	S	S	0	0
Magnesium Hydroxide		U	0	U	0	0	S	S	0	S	U	S	S	0	0	S	0	S	0
Magnesium Nitrate		M	0	0	0	0	0	0	0	S	0	Sd	S	0	0	0	0	0	0
Magnesium Sulphate		S	0	0	0	0	0	0	0	S	0	St	S	0	0	0	0	0	0
Manganese Salts		M	0	S	0	0	0	0	0	S	0	S	S	0	0	S	0	S	0
Mercury		0	0	0	0	0	0	0	0	S	U	S	S	S	0	0	0	0	0
Methanol (100%)		S	S	U	U	M	S	0	U	S	M	S	D	S	S	S	S	S	U
Methyl Acetate		S	0	0	0	0	0	0	0	M	U	M	M	U	0	0	0	0	0
Methyl Alcohol (100%)		S	S	U	U	M	S	0	U	S	M	S	D	S	S	S	S	S	U
Methyl Butyl Ketone		0	0	0	0	0	0	0	0	U	0	0	0	0	0	0	0	0	0
Methyl Ethyl Ketone		S	U	U	U	M	M	0	U	S	U	S	S	U	0	S	M	S	U
Methyl Isobutyl Ketone		St	0	0	0	0	0	0	0	S	U	S	S	U	0	0	0	0	0
Methyl Isopropyl Ketone		0	0	0	0	0	0	0	0	U	U	S	U	U	0	0	0	0	0
Methylene Chloride		X	U	U	U	S	S	0	U	U	U	M	U	U	S	S	S	S	M
Mineral Oil		0	0	0	0	0	0	0	0	Mt	U	Mt	Mt	Mt	0	0	0	0	0
Nickel Chloride		U	0	0	0	0	0	0	0	S	0	St	S	0	0	0	0	0	0
Nickel Salts		M	S	S	0	0	0	0	S	S	S	S	S	0	S	S	S	S	S

Chapter 6

Service and Maintenance

Chemical	Material	AL	BN	CAB	CN	DL	KY	NO	NY	PA	PC	PE	PP	PS	SS	TF	TZ	TI	VA
	PPCO																		
Nickel Sulphate	U	0	0	0	0	0	0	0	0	S	S	St	S	0	0	0	0	0	0
Nitric Acid (10%)	M	U	S	S	U	S	S	M	D	S	S	S	S	D	S	S	S	S	S
Nitric Acid (20%)	U	0	0	0	0	0	0	0	0	S	Sd	S	S	St	0	0	0	0	0
Nitric Acid (50%)	M	U	M	M	U	S	S	M	D	M	M	M	0	D	S	S	S	S	S
Nitric Acid (95%)	M	U	U	0	U	0	0	U	M	U	U	M	U	S	S	S	S	S	S
Nitric Acid (conc.)	St	0	0	0	0	0	0	0	U	U	Mt	U	U	0	0	0	0	0	0
Nitrobenzene	0	0	0	0	0	0	0	0	U	U	U	U	U	0	0	0	0	0	0
Octane	0	0	0	0	0	0	0	0	S	Sd	S	S	Sd	0	0	0	0	0	0
Octyl Alcohol	S	0	0	0	0	0	0	0	0	0	S	0	0	0	0	0	0	0	0
Oleic Acid	S	U	S	S	S	S	0	S	S	S	S	S	S	S	S	S	S	S	M
Orange Essence	S	0	0	0	0	0	0	0	Mt	M	Mt	Mt	M	0	0	0	0	0	0
Oxalic Acid	M	M	S	S	0	S	0	S	S	S	S	S	S	S	S	S	S	M	S
Oxygenated Water (20%)	S	0	0	0	0	0	0	0	S	S	S	S	S	0	0	0	0	0	0
Oxygenated Water (50%)	S	0	0	0	0	0	0	0	S	S	S	S	S	0	0	0	0	0	0
Oxygenated Water (90%)	S	0	0	0	0	0	0	0	S	S	S	S	S	0	0	0	0	0	0
Ozone	0	0	0	0	0	0	0	0	Sd	Sd	S	Sd	S	0	0	0	0	0	0
Paraffin	S	0	0	0	0	0	0	0	S	0	S	S	0	0	0	0	0	0	0
Pentane	S	0	0	0	0	0	0	0	U	0	U	U	0	0	0	0	0	0	0
Perchloroethylene	S	0	0	0	0	0	0	0	U	U	U	U	U	0	0	0	0	0	0
Perchloric Acid	X	0	0	0	0	0	0	0	St	U	St	St	U	0	0	0	0	0	0
Perchloric Acid (10%)	U	0	0	0	U	S	0	0	S	U	M	M	0	U	S	S	S	S	S
Perchloric Acid (70%)	X	0	0	0	0	0	0	0	M	U	M	M	U	0	S	S	0	0	0
Petrol	S	0	0	0	0	0	0	0	St	M	St	St	M	0	0	0	0	0	0
Phenol (5%)	S	U	0	0	U	S	0	U	M	U	S	M	U	S	S	S	U	S	S
Phenol (50%)	U	0	0	0	0	0	0	0	U	U	U	U	U	0	S	M	0	0	0
Phenol, crystals	U	0	0	0	0	0	0	0	St	U	St	St	U	0	0	0	0	0	0
Phenol, liquid	U	0	0	0	0	0	0	0	U	U	U	U	U	0	0	0	0	0	0
Phenyl Ethyl Alcohol	0	0	U	0	0	0	0	S	S	0	S	S	0	0	S	0	S	0	0
Phosphoric Acid (10%)	0	M	S	S	U	S	S	0	S	S	S	S	S	S	S	S	0	S	S
Phosphoric Acid (conc.)	0	U	M	M	U	S	0	0	S	U	S	S	S	M	S	S	M	S	S
Picric Acid	S	0	0	0	0	0	0	0	U	U	U	U	U	0	0	0	0	0	0
Pine Oil	0	0	0	0	0	0	0	0	Sd	St	St	Sd	M	0	0	0	0	0	0
Potash, conc.	U	0	0	0	0	0	0	0	S	U	S	S	S	0	0	0	0	0	0
Potassium Bromide	U	0	0	0	0	0	0	0	S	S	S	S	0	0	0	0	0	0	0
Potassium Carbonate	M	0	S	S	0	S	S	S	S	U	S	S	0	S	S	S	S	0	0
Potassium Chlorate	M	0	S	S	0	S	S	S	S	S	S	S	0	S	S	0	S	0	0
Potassium Chloride	U	0	0	0	0	0	0	0	S	S	S	S	S	0	S	S	0	0	0
Potassium Hydroxide (5%)	U	M	S	M	U	0	0	S	S	U	S	S	S	S	S	S	M	S	S
Potassium Hydroxide (conc.)	U	M	U	U	U	0	0	0	S	U	S	S	0	S	S	S	U	M	M
Potassium Nitrate	S	0	0	0	0	0	0	0	S	0	S	S	0	0	0	0	0	0	0
Potassium Permanganate	S	0	0	0	0	0	0	0	S	S	S	S	D	0	S	S	0	0	0
Propane Gas	S	0	0	0	0	0	0	0	U	St	U	U	M	0	0	0	0	0	0
Propionic Acid	0	0	0	0	0	0	0	0	Sd	U	M	Sd	S	0	0	0	0	0	0
Propyl Alcohol	S	0	0	0	0	0	0	0	S	0	St	S	0	0	0	0	0	0	0
Propylene Glycol	S	0	0	0	0	0	0	0	S	Sd	S	S	S	0	0	0	0	0	0
Propylene Oxide	0	0	0	0	0	0	0	0	S	St	S	S	S	0	0	0	0	0	0
Pyridine	U	0	0	0	0	0	0	0	M	U	S	M	0	0	0	0	0	0	0
Resorcinol, Sat'd., Sol	0	0	0	0	0	0	0	0	S	Sd	S	S	U	0	0	0	0	0	0

Chemical	Material	AL	BN	CAB	CN	DL	KY	NO	NY	PA	PC	PE	PP	PS	SS	TF	TZ	TI	VA
		PPCO																	
Rubidium Bromide	M	0	0	0	0	0	0	0	0	S	S	0	S	0	0	0	0	0	0
Saccharose	U	0	0	0	0	0	0	0	0	S	S	S	S	S	0	0	0	0	0
Salicylic Acid, Sat	0	0	0	0	0	0	0	0	0	S	Sd	S	S	S	0	0	0	0	0
Serum	S	0	0	0	0	0	0	0	0	S	S	S	S	S	0	S	S	0	0
Silver Acetate	0	0	0	0	0	0	0	0	0	S	Sd	S	S	S	0	0	0	0	0
Silver Nitrate	U	0	0	0	0	0	0	0	0	S	S	S	S	S	0	S	S	0	0
Sodium Acetate	S	0	0	0	0	0	0	0	0	S	Sd	S	S	S	0	0	0	0	0
Sodium Bisulphate	M	0	S	S	0	S	S	S	S	S	S	S	0	S	S	0	S	0	0
Sodium Borate	M	0	0	0	0	0	0	0	0	S	S	Sd	S	0	0	0	0	0	0
Sodium Bromide	U	0	0	0	0	0	0	0	0	S	S	0	S	0	0	0	0	0	0
Sodium Carbonate (2%)	M	S	S	S	S	S	S	S	S	S	S	D	0	S	S	S	S	S	S
Sodium Chloride (10%)	S	S	S	S	S	0	0	S	S	S	S	S	S	S	S	S	S	M	S
Sodium Chloride (Sat'd.)	S	S	0	0	S	0	0	S	S	0	S	S	0	S	S	S	S	S	S
Sodium Hydroxide (>1%)	U	M	S	S	U	S	0	S	S	U	S	S	S	S	S	S	S	S	S
Sodium Hydroxide (10%)	U	M	U	U	U	S	0	S	S	U	S	S	S	S	S	S	S	S	S
Sodium Hydroxide (conc.)	U	M	U	U	U	0	0	0	M	U	S	M	0	S	S	S	M	U	0
Sodium Hypochlorite (5%)	M	M	S	S	U	S	S	S	D	S	S	S	S	M	S	S	S	S	S
Sodium Iodide	M	0	0	0	0	0	0	0	0	S	S	0	S	0	0	0	0	0	0
Sodium Nitrate	S	0	0	0	0	0	0	0	0	S	0	Sd	S	0	0	0	0	0	0
Sodium Sulfate	S	0	0	0	0	0	0	0	0	Sd	0	Sd	Sd	0	0	0	0	0	0
Sodium Sulphide	S	S	S	0	0	S	0	S	S	U	S	S	0	S	S	S	M	S	S
Stearic Acid	S	0	0	0	0	0	0	0	0	S	Sd	S	S	S	0	0	0	0	0
Sulphuric Acid (10%)	M	U	S	S	U	S	S	S	S	M	S	S	S	U	S	S	S	S	S
Sulphuric Acid (20%)	U	0	0	0	0	0	0	0	0	Sd	Sd	S	Sd	S	0	0	0	0	0
Sulphuric Acid (50%)	U	U	U	U	U	S	S	U	S	S	S	S	S	U	S	S	M	S	S
Sulphuric Acid (conc.)	U	U	U	U	U	S	0	U	D	U	M	D	U	M	S	S	U	S	S
Sulphuric Anhydride, dry or moist	S	0	0	0	0	0	0	0	0	S	Sd	S	S	S	0	0	0	0	0
Tetrachloroethane	M	0	0	0	0	0	0	0	0	M	0	0	M	0	0	0	0	0	0
Tetrachlorethylene	0	0	0	0	0	0	0	0	0	U	0	S	U	0	0	0	0	0	0
Tannic Acid	M	0	0	0	0	0	0	0	0	S	0	Sd	S	0	0	0	0	0	0
Tartaric Acid	M	0	0	0	0	0	0	0	0	S	Sd	S	S	S	0	0	0	0	0
Tetrahydrofuran	S	0	0	0	0	0	0	0	0	U	U	U	U	U	0	S	S	0	0
Thionyl Chloride	0	0	0	0	0	0	0	0	0	U	U	U	U	U	0	0	0	0	0
Toluene	S	U	P	S	M	S	0	U	U	U	U	U	U	S	S	S	M	M	0
Trichlorethylene	S	U	0	0	0	S	0	U	U	U	U	U	U	U	S	S	M	S	S
Trichloroacetic Acid	U	0	0	0	0	0	0	0	0	Mt	Mt	Mt	Mt	S	0	0	0	0	0
1,2,4 - Trichlorobenzen	0	0	0	0	0	0	0	0	0	U	U	U	U	U	0	0	0	0	0
Trichloroethane	S	U	S	0	M	S	0	S	U	U	U	U	M	0	S	S	S	S	S
Triethylamine	0	0	0	0	0	0	0	0	0	U	0	0	U	0	0	0	0	0	0
Triethylene Glycol	0	0	0	0	0	0	0	0	0	S	Sd	S	S	S	0	0	0	0	0
Tris Buffer (neutral)	S	0	0	0	0	0	0	0	0	S	S	S	S	S	0	S	S	0	0
Trisodium Phosphate	0	0	S	0	M	0	0	S	S	0	S	S	0	0	S	S	S	S	S
Triton X-100	S	0	0	0	0	0	0	0	0	S	S	S	S	S	0	S	M	0	0
Turpentine	S	0	0	0	0	0	0	0	0	Sd	Mt	St	Sd	U	0	0	0	0	0
Undecyl Alcohol	0	0	0	0	0	0	0	0	0	Sd	Sd	St	Sd	M	0	0	0	0	0
Urea	M	0	S	S	S	0	0	S	S	S	S	S	S	S	S	S	S	S	0
Urine	0	0	S	0	S	0	0	S	S	S	S	S	0	0	S	S	S	0	0
Vinylidene chloride	0	0	0	0	0	0	0	0	0	U	U	U	U	U	0	0	0	0	0

Chapter 6

Service and Maintenance

Chemical	Material	AL	BN	CAB	CN	DL	KY	NO	NY	PA	PC	PE	PP	PS	SS	TF	TZ	TI	VA
		PPCO																	
Xylene		S	U	P	O	M	S	O	U	U	U	U	U	U	S	S	S	S	S
Zinc Chloride		M	S	S	O	O	O	O	S	S	S	S	S	S	M	S	S	S	S
Zinc Hydrosulphite		U	O	O	O	O	O	O	O	O	O	O	O	O	O	O	O	O	O
Zinc Sulphate		U	O	O	O	O	O	O	O	Sd	O	S	Sd	O	O	O	O	O	O

* This table is intended as a guide only because of the difficulty in quantifying, cross-checking and monitoring the results under different conditions of temperature, pressure and purity relating to the solvents and samples dissolved therein. It is strongly recommended that you carry out your own trials, particularly before protracted work periods.

Chapter 7 Disposal of Product

The following disposal recommendations are valid for the machine (or its accessories) at the end of its useful life, or the parts that be disposed of because they are worn out or degraded during use.

Prior to disposal, the machine and accessories must be decontaminated. In this respect the user is required to submit the enclosed decontamination certificate, completed and signed, to the company or persons who are in charge of disposal.

The elements of the product that may become noxious during the life of the product are the following:

- Electric batteries and accumulators situated in the front panel of the machine among the other electrical and electronic components,
- Oil in the compressor of the refrigeration systems,
- Refrigerant

Disposal of these elements must be in accordance with applicable regulations and recommendations defined by the relevant regulatory bodies. In addition, these elements must be disposed of differently based on the different noxious substances they contain (possibly by a specialized disposal company).

Certificate of Decontamination and Cleaning



Read carefully the instructions below before sending an instrument, or parts of it, to Thermo Service Dept. or to any Authorized Technical Assistance Service. ▲

Mr / Mrs (name) Establishment

Department

Address Post / Zip code

City State / Country

Declares the cleaning and decontamination of the following:

Product type Serial N°

Rotor Serial N°

Rotor Serial N°

Accessory - Description Serial N°

Accessory - Description Serial N°

Nature of contamination

.....
.....

Decontamination Procedure used

.....
.....

Decontamination certified by:

Mr / Mrs Institution

Date Signature

When an instrument, or parts of it, requires servicing by Thermo personnel, the following procedure must be accomplished to ensure personnel safety:

- Clean the instrument and proceed to its decontamination from any kind of dangerous products.
- Compile this Decontamination Certificate with all the information required.

- Attach this Certificate to the instrument (or part) before sending it to Thermo Service or other authorized technical service.

Thermo personnel will not accept to work on instruments deprived of this Decontamination Certificate.

If an instrument is received at our Service facilities and, in our opinion, is a radioactive or biological hazard, the item will be refused and resent to the Customer. Disposition costs will be borne by the sender.

Instructions for decontamination and cleaning are explained in the User Manual. Additional certificates are available from your local technical or Customer Service representative. In the event these certificates are not available, a written statement certifying that the instrument or part has been properly decontaminated and outlining the procedures used will be acceptable.

For your convenience, use a copy of this page

