

Convex Array Probe

EUP-C514

INSTRUCTION MANUAL

Notes for operators and responsible maintenance personnel

- ★ Please read through this Instruction Manual carefully prior to use.
- ★ Keep this Instruction Manual together with the system with care to make it available anytime.

 **Hitachi, Ltd.**

Tokyo, Japan

Q1E-EP0428-10

© Hitachi, Ltd. 2013,2017. All rights reserved.

 0123

Manufacturer:



Hitachi, Ltd.
2-16-1, Higashi-Ueno, Taito-ku, Tokyo, 110-0015,
Japan
+81-3-6284-3668
[http://www.hitachi.com/businesses/healthcare/
index.html](http://www.hitachi.com/businesses/healthcare/index.html)

European
Representative:



Hitachi Medical Systems GmbH
Otto-von-Guericke-Ring 3 D-65205 Wiesbaden,
Germany

EU Importer: Hitachi Medical Systems Europe Holding AG
Address: Sumpfstrasse 13 CH-6300 Zug, Switzerland

Local Distributor:

About this manual

This instruction manual shall provide instructions for using, cleaning, disinfecting and/or sterilizing the HITACHI ultrasound probe. It also describes safety considerations, maintenance.

For instructions for operating the main unit, refer to the operation manual for it.

Before using the probe, thoroughly read this manual and keep this book for future reference.

If you have any questions concerning the manual, please contact a service support.

The following conventions are used throughout the manual to denote information of special emphasis.




WARNING: "Warning" is used to indicate the presence of a hazard which can cause severe personal injury, death, or substantial property damage if the warning is ignored.

CAUTION: "Caution" is used to indicate the presence of a hazard which will or can cause minor personal injury or property damage if the caution is ignored.

NOTICE: "Notice" is used to notify people of installation, operation, or maintenance information which is important, but not hazard related.










Graphical Symbols for Use in Labeling of Hitachi Ultrasound Probes

Some graphical symbols that are used in labeling of Hitachi Ultrasound Probes are compliant with EN980:2008 standard. Refer to the following table about the meanings of them.

Explanation of Symbol	Symbol	Descriptive Content
Manufacturer Company Name and Address		Hitachi, Ltd. 2-16-1, Higashi-Ueno, Taito-ku, Tokyo, 110-0015, Japan +81-3-6284-3668 http://www.hitachi.com/businesses/healthcare/index.html
Authorized Representative in The European Community		Hitachi Medical Systems GmbH Otto-von-Guericke-Ring 3 D-65205 Wiesbaden, Germany
Keep away from Sunlight		Store the probe in a cool, dustproof and dark, dry place to avoid high temperature, humidity and direct sunlight.

Definition of symbol

The following symbol is also used for HITACHI Ultrasound Probes.

Location	Symbol	Definition
Probe connector		This instrument complies with Directive 93/42/EEC relating to Medical Device and Directive 2011/65/EU relating to RoHS
Probe connector	IPX7	IPX7 mark See section 1.7.
Probe connector		Type BF APPLIED PART
Probe connector		General warning sign
Probe connector		Warning; dangerous voltage
Probe connector		Caution; Biohazard
Probe connector		Follow the instruction manual to operate this instrument. If not avoided, may result in injury, property damage, or the equipment trouble.
Probe connector		STERRAD sterilization compatibility mark
Probe connector		Upper Limit of Temperature; The probes that are <u>applicable</u> to Ethylene Oxide Gas Sterilization use symbol of “Upper Limit of Temperature: 55 degrees”.
Probe connector		Do not waste the instrument as general waste. Comply with a local regulation.
Probe connector	Rx Only	By prescription only. U.S. Federal Law restricts this device to sale on order of a physician only.

CONTENTS

	Page
1. General	1
1.1. General	1
1.2. Principles of operation	1
1.3. Intended Use	2
1.4. Composition	2
1.5. Option	3
1.6. Option of Hitachi ultrasound diagnostic scanner	3
1.7. External View	4
2. Inspection before Use	5
2.1. Inspection for Appropriate Connection	5
2.2. Inspection for Material Surface	5
3. Operation Procedure	6
4. Option of Hitachi ultrasound diagnostic sensor	7
4.1. Magnetic Sensor (EZU-RV2S)	7
4.2. Magnetic Sensor (EZU-RV3S)	10
5. Reprocessing Procedure	13
5.1. Point of use (Pre-cleaning)	15
5.2. Containment and transportation	15
5.3. Manual Cleaning and disinfection	15
5.4. Drying	18
5.5. Inspection	18
5.6. Packaging	18
5.7. Sterilization	18
5.8. Storage	20
6. Maintenance and Safety Inspection	21
7. Safety Precautions	22
8. Specification	23
8.1. Probe	23
8.2. Suppliers List	24
9. Disposal of the probe	24

1. General

1.1. General

The EUP-C514 is a convex array probe.

The acoustic output of the EUP-C514 was measured according to the IEC60601-2-37 standard and the measurement was conducted by operating with the Hitachi ultrasound diagnostic scanner.

The measured acoustic output is listed in the instruction manual of the Hitachi ultrasound diagnostic scanner.

The EUP-C514 is categorized in class IIa according to Directive 93/42/EEC and classified as type BF according to IEC60601-1.

1.2. Principles of operation

This probe and the ultrasound diagnostic scanner enable image diagnosis using ultrasonic waves. This system operates under the principles described below.

- 1) When an electric pulse signal is applied from the transmitter to the transducer of the probe, the transducer converts electric signals into mechanical vibration energy for emitting pulse-shaped ultrasonic waves into the body part, liquid or other medium contacting the transducer.
- 2) The emitted ultrasonic waves are reflected by boundaries with different acoustic characteristics (acoustic impedance) within the body.
- 3) The transducer is also used to receive reflected ultrasonic waves. The transducer vibrates mechanically due to the received ultrasonic waves and converts mechanical vibrations into electric energy. Electric signals are converted to shades of brightness by brightness modulation to obtain an image.

1.3. Intended Use

The EUP-C514 is designed for observation and diagnosis mainly of the following regions by connecting with the Hitachi ultrasound diagnostic scanner.

- General abdominal organs
- General OB/GYN organs
- Biopsy (with Biopsy Attachment)

〈WARNING〉

Never use the probe for following applications.

- Direct contact to the heart.
- Biopsy to the heart.

1.4. Composition

The components of the EUP-C514 are given follows:

- 1) Probe EUP-C514 1 piece
- 2) Instruction Manual 1 copy

〈CAUTION〉

Sterilization has not been made to the probe, shipped from the factory. Prior to use of the probe, be sure to clean and sterilize the probe.

1.5. Option

1.5.1. Biopsy Attachment EZU-PA34T

The biopsy attachment EZU-PA34T is a dedicated tool for use as mounted on a EUP-C514. The optional biopsy attachment EZU-PA34T components are as follows:

- 1) Biopsy guide assembly ······ 1 piece
- 2) Needle guide
(14G, 18G and 21G) ······ 1 each
- 3) Brush ······ 1 piece
- 4) Instruction manual ······ 1 copy
- 5) Biopsy case ······ 1 piece

Please refer to the instruction manual of option about the method of handling, cleaning and sterilizing the biopsy attachment EZU-PA34T.

1.5.2. Needle Guide Bracket EZU-PA5C1

- 1) Needle guide bracket ······ 1 piece
- 2) Brush ······ 1 piece
- 3) Spring (Spare) ······ 2 pieces
- 4) Instruction manual ······ 1 copy
- 5) Biopsy case ······ 1 piece

Please refer to the instruction manual of option about the method of handling, cleaning and sterilizing the needle guide bracket EZU-PA5C1.

1.6. Option of Hitachi ultrasound diagnostic scanner

1.6.1. Magnetic Sensor Attachment


- 1) Magnetic sensor attachment
- 2) Spacer for EZU-RV2S

Please refer to this instruction manual about the method of handling, cleaning and sterilizing the Magnetic sensor attachment.

〈 CAUTION 〉

The probe has not been sterilized when it was shipped from a factory. So before using the probe, clean, disinfect and if necessary sterilize the probe certainly.

1.7. External View

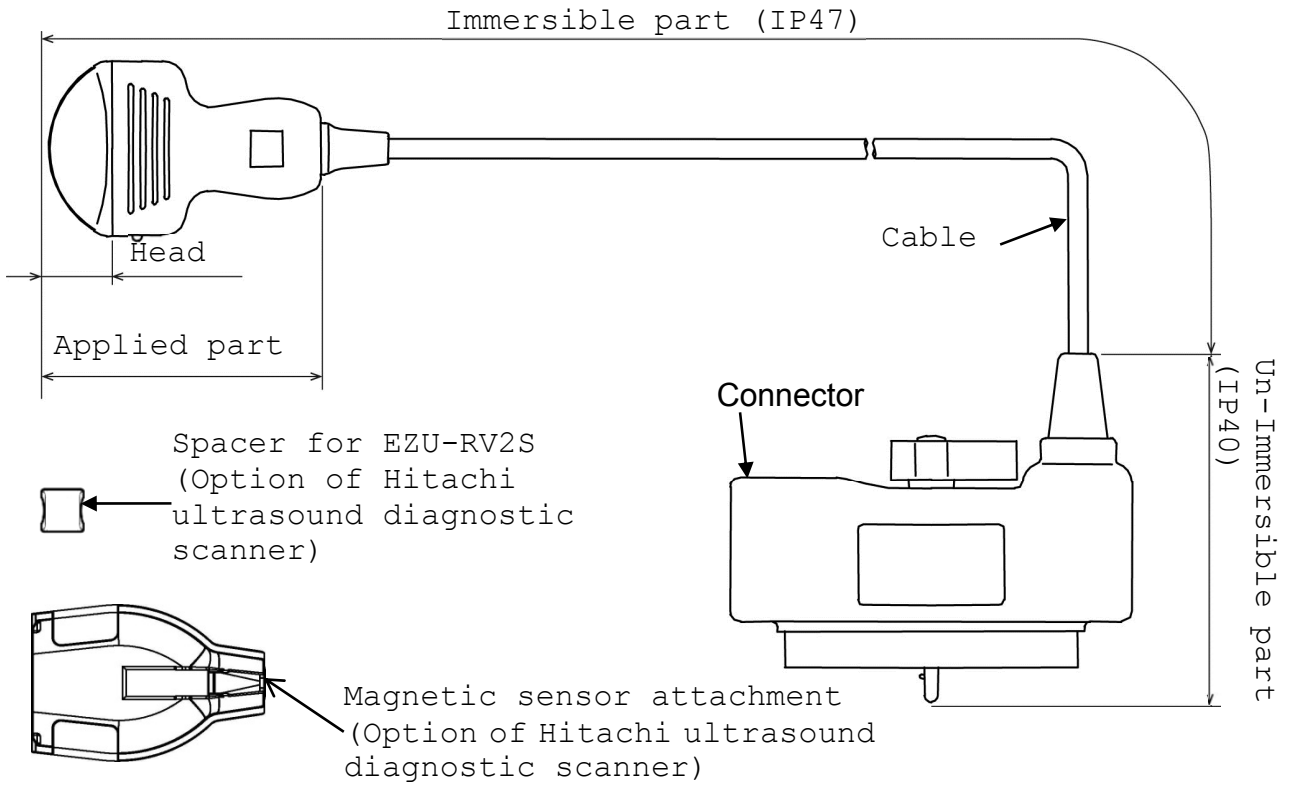

Immersible part: This part can be immersed in disinfectant solution and also can be cleaned by water.

Un-immersible part: This part should not be immersed in disinfectant solution and also cannot be cleaned by water.

Fig. 1 External View

2. Inspection before Use

Prior to use, the probe must be carefully inspected that it is appropriate for use. If you find any damage, do not use the probe and immediately contact a service support.

2.1. Inspection for Appropriate Connection

- 1) Confirm that the system is correctly operating. Refer to the instruction manual for the ultrasound diagnostic scanner.
- 2) Do not attach or connect unauthorized devices or instruments on the probe, such as unauthorized biopsy attachments. If a biopsy operation is required, refer to its instruction manual for inspection, preparation, operation and cleaning through sterilization.

2.2. Inspection for Material Surface

- 1) Visually inspect the surface of the probe and head, housing, the cable and the connector for any crack, scratch or denaturalization.
- 2) Visually inspect the Magnetic sensor attachment and the Spacer for EZU-RV2S for any crack, deformation, or denaturalization.

3. Operation Procedure

- 1) Confirm that the probe is cleaned, disinfected and if necessary sterilized.
- 2) Confirm that the Magnetic sensor attachment and the Spacer for EZU-RV2S is disinfected or sterilized, when use RVS (Real-time Virtual Sonography).
- 3) Connect the probe to the ultrasound diagnostic scanner, operate the scanner, and adjust the image, all according to the instructions given in the operation manual for the ultrasound diagnostic scanner with which the probe is used as connected.
- 4) Confirm the direction of the probe. The relationship between the direction of the probe and image is shown in Fig. 2. The Right-left orientation mark on the image indicates the direction of the index mark of the probe.

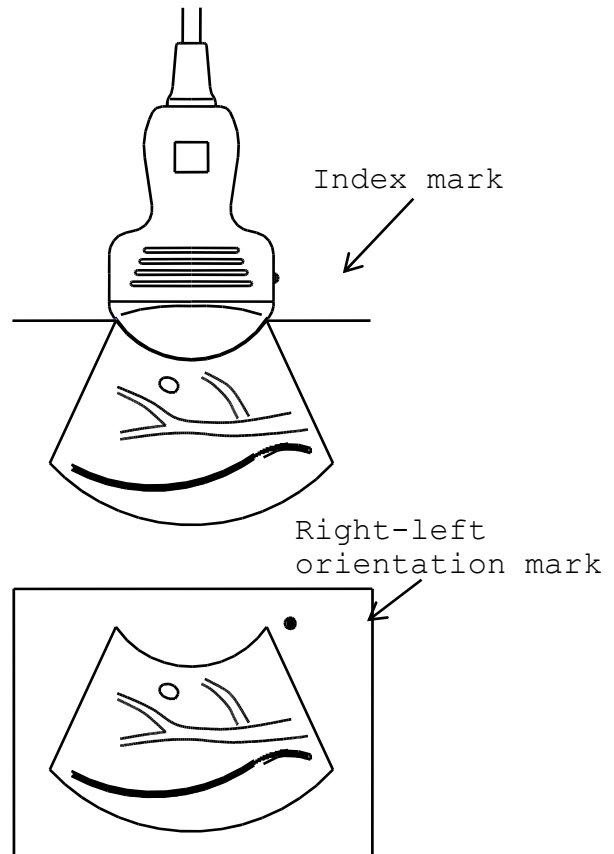


Fig. 2 Relationship between the directions of the probe and the Right-left orientation mark

- 5) If a biopsy method is required, refer to its instruction manual.
- 6) Under sterile condition, protecting the probe by using covers is recommended. Some Latex material may create allergic reaction. Please use allergy free material covers.
- 7) After using the probe, perform the reprocessing procedure in accordance with the procedure stated in “5. Reprocessing procedure of the probe” every time immediately after completing the ultrasound examination.
- 8) After using the Magnetic sensor attachment and the Spacer for EZU-RV2S, perform the reprocessing procedure in accordance with the procedure stated in “6. Reprocessing procedure of the Magnetic Sensor Attachment and the Spacer for EZU-RV2S” every time immediately after completing the ultrasound examination.
- 9) Store the Magnetic sensor attachment and the Spacer for EZU-RV2S in the environment indicated in “7.Maintenance and Safety inspection”.

4. Option of Hitachi ultrasound diagnostic sensor


In case of using RVS (Real-time Virtual Sonography), confirm that type of the Magnetic sensor. There are two types of magnetic sensors for the EUP-C514, the EZU-RV2S and the EZU-RV3S.

The Magnetic sensor (EZU-RV2S) and the Magnetic sensor (EZU-RV3S) are shown in Fig. 3 and Fig.8.

The use of the EUP-C514 with either of the magnetic sensors enables the user to perform RVS (Real-time Virtual Sonography).

4.1. Magnetic Sensor (EZU-RV2S)

The Magnetic sensor (EZU-RV2S) as shown in Fig.3 is a magnetic sensor for the EUP-C514.

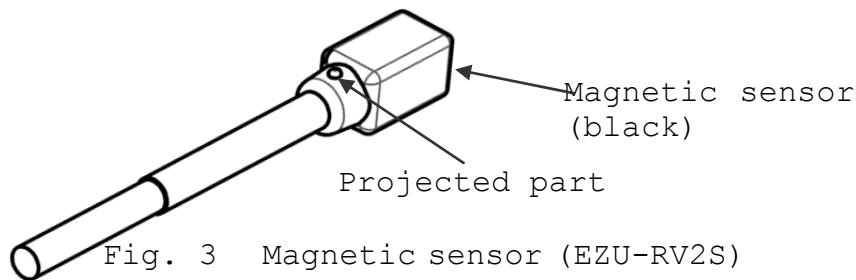

4.1.1. How to attach the Magnetic Sensor

The Procedure of attaching the Magnetic sensor is as follows.

- 1) Confirm that the probe, the Magnetic sensor attachment and the Spacer for EZU-RV2S are disinfected or sterilized.
- 2) Connect the probe, operate the ultrasound diagnostic scanner, and adjust the image according to the instructions given in the operation manual for the ultrasound diagnostic scanner.
- 3) To use Real-time Virtual Sonography (RVS), attach the Magnetic sensor as shown below.

- a) Attach the Spacer for EZU-RV2S to the Magnetic sensor.
- b) Insert the Magnetic sensor (EZU-RV2S) into the Magnetic sensor attachment with the correct direction as shown in Fig. 4.

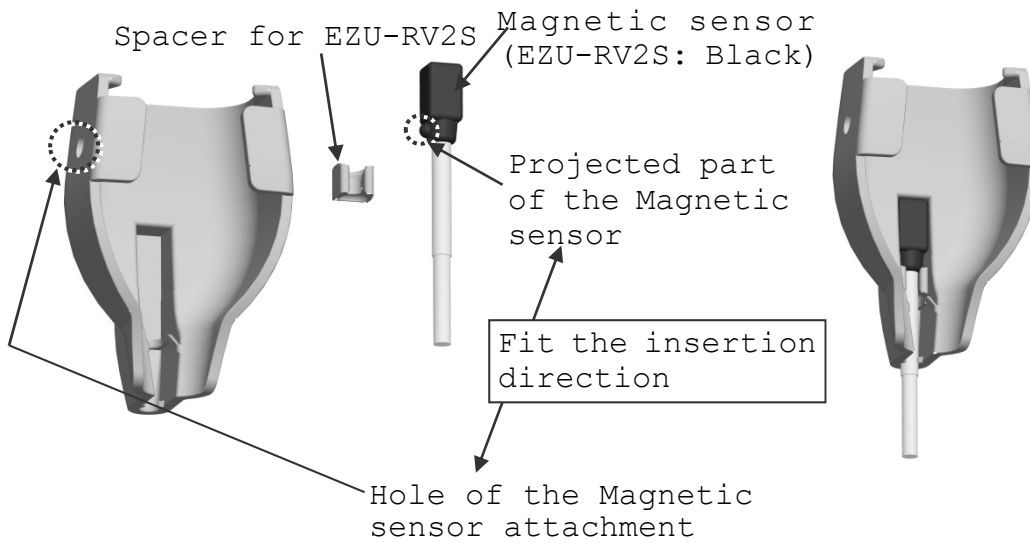


Fig. 4 How to attach the Magnetic sensor

- c) Place the Magnetic sensor attachment in the index mark of the probe.

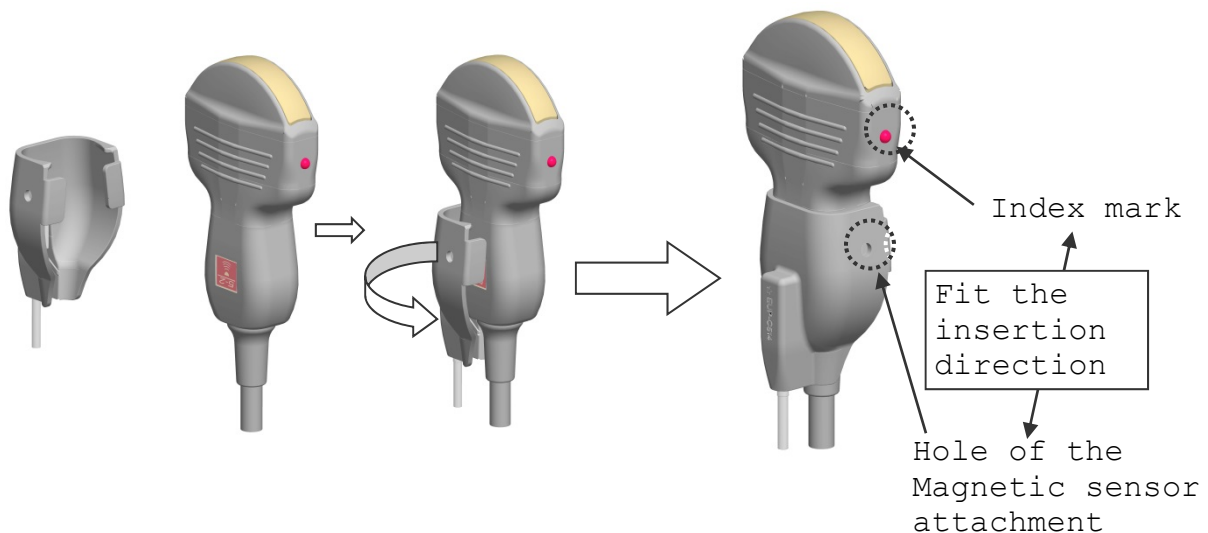


Fig. 5 How to attach the Magnetic sensor attachment

< CAUTION >

- Never attach the Magnetic sensor attachment to the probe in the incorrect direction, otherwise it may result false diagnosis.
- Never forget to attach the Spacer for EZU-RV2S to the Magnetic sensor, otherwise it may result in false diagnosis.

4.1.2. How to release the Magnetic Sensor

The procedure of releasing the Magnetic sensor from the probe is as follow.

- 1) Turn around the Magnetic sensor attachment and release it from the probe as shown in Fig. 6.

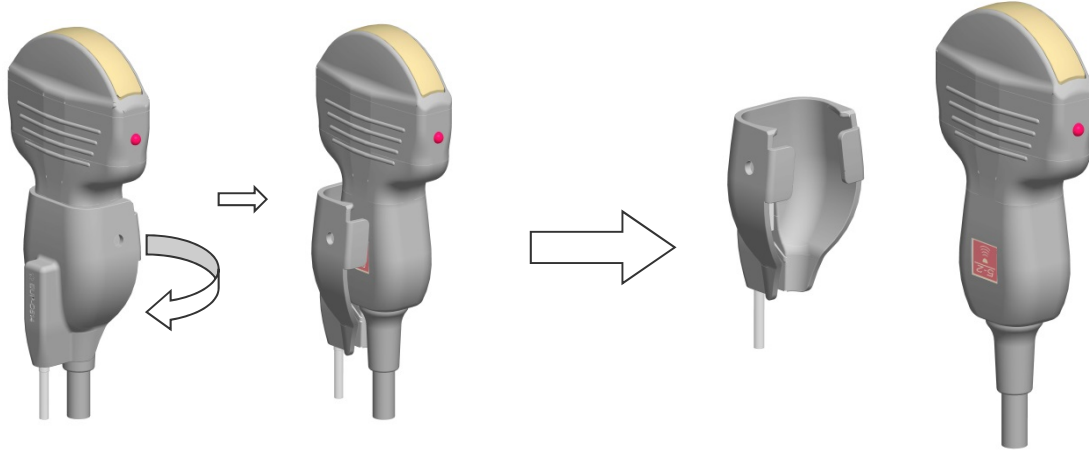


Fig. 6 How to release the Magnetic sensor attachment

- 2) Release the Magnetic sensor from the Magnetic sensor attachment as shown in Fig. 7 and release the Spacer for EZU-RV2S from the Magnetic sensor.

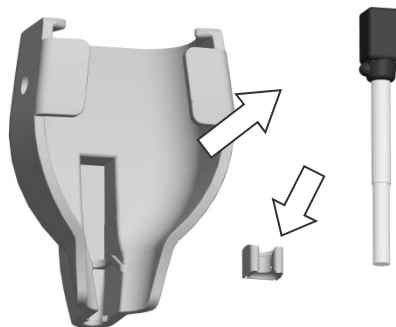


Fig. 7 How to release the Magnetic sensor

〈 CAUTION 〉

The Spacer for EZU-RV2S is small, so please do not lose the spacer.

4.2. Magnetic Sensor (EZU-RV3S)

The Magnetic sensor (EZU-RV3) as shown in Fig. 8 is also the Magnetic sensor for the EUP-C514.

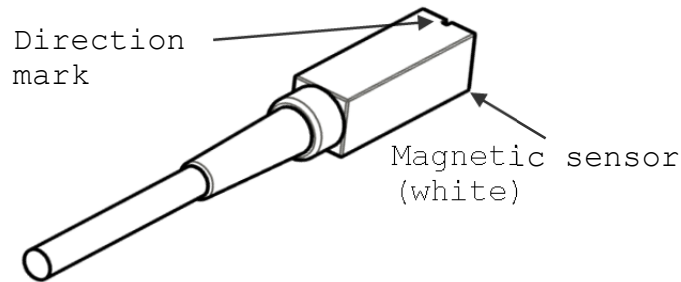


Fig. 8 Magnetic sensor (EZU-RV3S)

4.2.1. How to attach the Magnetic Sensor

The procedure of attaching the Magnetic sensor is as follows.

- 1) Confirm that the probe, the Magnetic sensor attachments are disinfected or sterilized.
- 2) Connect the probe, operate the ultrasound diagnostic scanner, and adjust the image according to the instructions given in the operation manual for the ultrasound diagnostic scanner.
- 3) To use Real-time Virtual Sonography (RVS), attach the magnetic sensor as shown below.
 - a) Attach the Magnetic sensor into the probe with the correct direction as shown in Fig. 9.

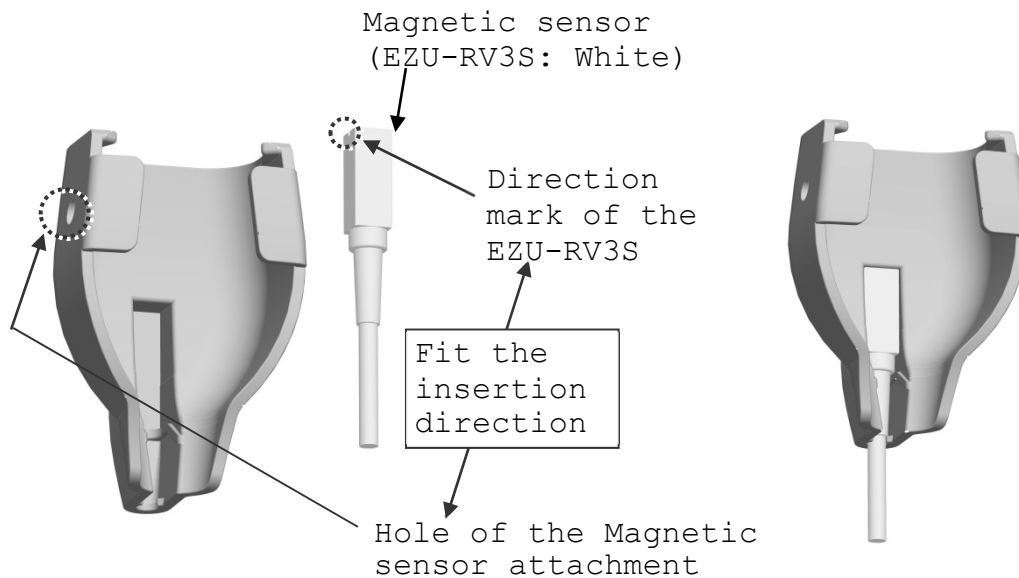


Fig. 9 How to attach the Magnetic sensor

- b) Place the Magnetic sensor attachment on the probe as shown in Fig. 10. Fit the projected part of the Magnetic sensor attachment in the index mark of the probe.

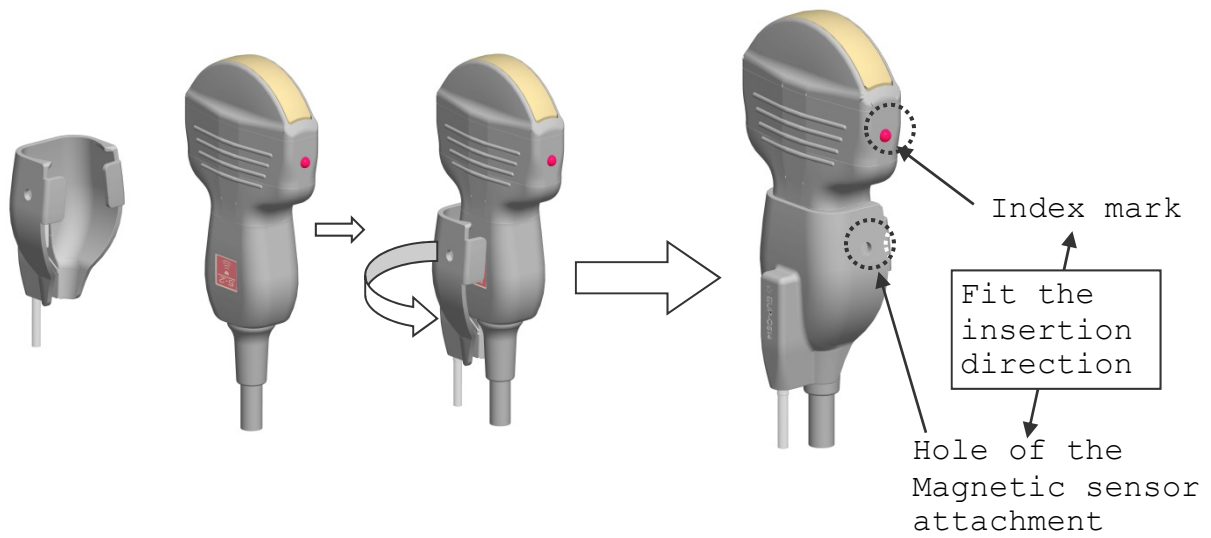


Fig. 10 How to attach the Magnetic sensor attachment

〈 CAUTION 〉

Never attach the Magnetic sensor attachment to the probe in the incorrect direction, otherwise it may result in false diagnosis.

4.2.2. How to release the Magnetic Sensor

The procedure of releasing the Magnetic sensor from the probe is as follow.

- 1) Turn around the Magnetic sensor attachment and release it from probe as shown in Fig. 11.

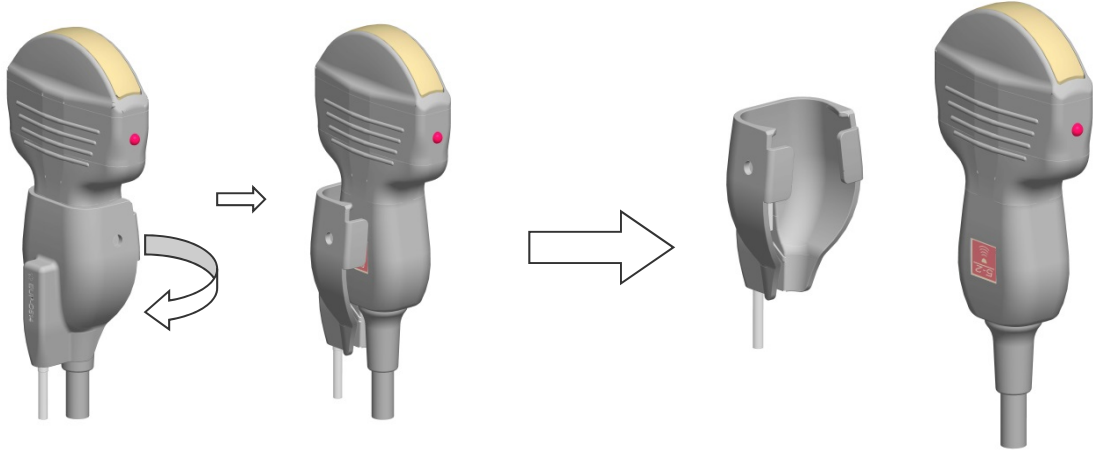


Fig. 11 How to release the Magnetic sensor attachment

- 2) Release the Magnetic sensor from the Magnetic sensor attachment as shown in Fig. 12.

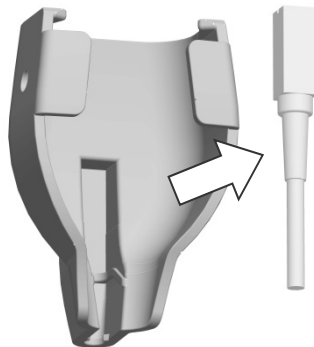


Fig. 12 How to release the Magnetic sensor

5. Reprocessing Procedure



The probe and accessory must be reprocessed after each use. Refer to the reprocessing instruction in this chapter.


WARNINGS	<ul style="list-style-type: none"> ➤ The probe is delivered unsterile. Prior to the first use, reprocess the probe. ➤ Temperature should not exceed 60°C during reprocessing. ➤ Probe connector is not water resistant.
Limitations on reprocessing	The probe is not completely submersible. The immersible part is shown in Fig.1. The un-immersible part should be disinfected by wipe disinfection.
Transportation before using	The probe should be packed in a sterile pouch or container to transport from Central Sterile Supply Department (CSSD) to an operating room. Be careful not to damage the sterile pouch or container during transportation.

Levels of reprocessing requirements:

Depending on the application of the product and with regard to risk evaluation, the user has to classify the medical device according to the current Medical Device Directive for processing of medical devices as uncritical, semi-critical or critical. Supporting information concerning this topic is listed in the table below. The user is responsible for correct classification of the medical device.

Classification	Definition	Processing
uncritical	Application part only contacts intact and uninjured skin	Cleaning Disinfection
semicritical	Application part contacts mucosa (intracavitary application)	Cleaning Disinfection (Disinfectant with virucidal effect)
critical	Application part contacts intracorporeal tissue directly (operative application)	Cleaning Disinfection (Disinfectant with virucidal effect - minimum) Sterilization

The flowchart of the reprocessing process of this probe is as follows.

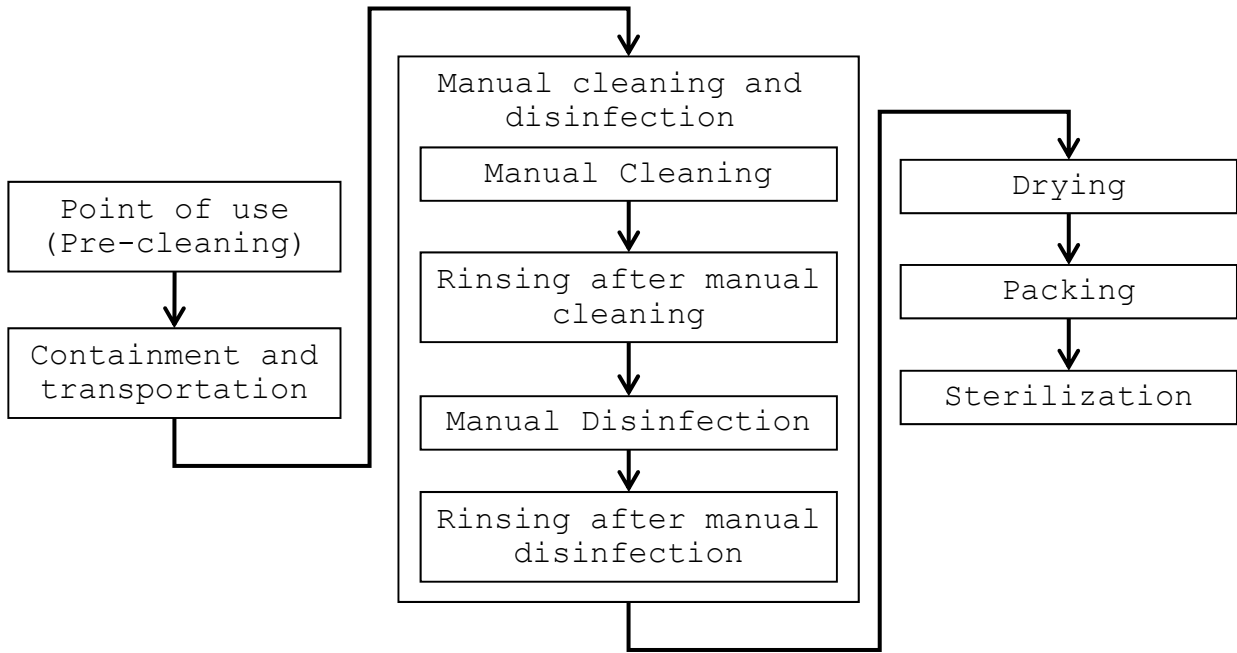

Point of use
(Pre-cleaning)

5.1. Point of use (Pre-cleaning)

Pre-cleaning should be done immediately after each use. The procedure is as follows:

A) EUP-C514 probe

- 1) Remove the protective cover.
- 2) Clean the probe of all patient's blood or fluid with running tap water until the surface of the probe looks visually clean.
- 3) Wipe the whole surface of the probe with gauze pad and remove superficial visible impurities.

B) Magnetic sensor Attachment

- 1) Remove the Attachment and the magnetic sensor from the probe.
- 2) Immerse the Attachment in sufficient amount of high quality tap water. Scrub it using soft cloth to remove all visible soil and from its surface.


Containment and
transportation

5.2. Containment and transportation

Putting the contaminated equipment into exclusive shock and damage proof container for transportation is recommended. It is recommended that instruments are reprocessed as soon as possible and not later than 4 hours after usage.

5.3. Manual Cleaning and disinfection

- a) Prepare following items before manual cleaning and disinfection:
- b) Detergent: Cidezyme® (Johnson & Johnson, #2258) or another cleaning agent with approved material compatibility for this medical device.
- c) Disinfectant: Cidex® OPA (Johnson & Johnson, # 20391) or another disinfectant with approved material compatibility for this medical device.
- d) Two tanks, one for cleaning and one for disinfection - optional: 1 additional tank for rinsing with deionized/tap water (sufficient size for immersion of the submergible part of the probe at full length)
- e) Soft, fluff free cloth or single use towel
- f) Personal protective equipment (gloves, water repellent protective skirt, face protection mask or protective glasses, see also instructions of the manufacturer for the detergent and the disinfectant)

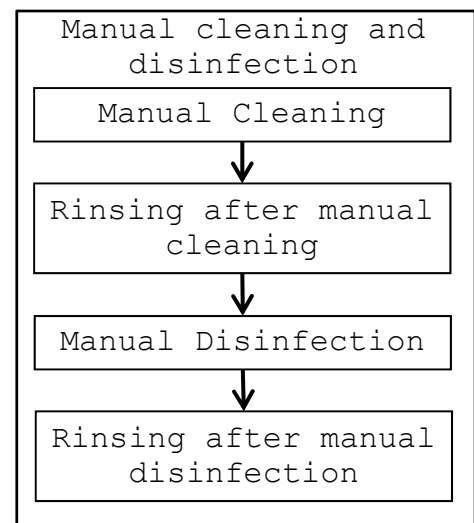

Manual Cleaning:

Prepare the detergent solution in a tank with cold water (please follow the instructions of the detergent manufacturer regarding application, dilution and contact time).

A) EUP-C514 probe

- 1) The temperature of the detergent solution should be between 15-30 °C, concentration is 1.6%. Please note the minimum contact time of the detergent in the manufacturer's instruction. If a differing detergent is used, please also note the approved material compatibility for the medical device.
- 2) Immerse the immersible part of the probe without connector into the diluted detergent solution (see Fig. 13). Wipe the immersible part of the probe under the surface of the detergent solution with a soft cloth to remove all visible soil. Be sure that all grooves of the probe are implemented during the cleaning process.
- 3) The immersible part of the probe should be left in the detergent solution according to the specified contact time of the detergent manufacturer.
- 4) Wipe the un-immersible parts of the probe with a soft cloth dipped with the detergent solution.
- 5) Rinse the probe with running tap water for 1 minute. (alternatively: immerse the immersible part of the probe in a tray filled with deionized water/tap water (see Fig. 13) for 5 min.)
- 6) Visually check the outer surface of the probe for cleanness. If necessary, use magnifying glass for visually check. If there is still soil visible, repeat all above steps.

B) Magnetic Sensor Attachment

- 1) The temperature of the detergent solution should be between 15-30 °C, concentration is 1.6%. Please note the minimum contact time of the detergent in the manufacturer's instruction. If a differing detergent is used, please also note the approved material compatibility for the medical device.
- 2) Immerse the Attachment into the diluted detergent solution. Wipe it under the surface of the detergent solution with a soft cloth to remove all visible soil. Be sure that all grooves of the attachment are implemented during the cleaning process.
- 3) The Attachment should be left in the detergent solution according to the specified contact time of the detergent manufacturer.
- 4) Rinse the Attachment with running tap water for 1 minute. (alternatively: immerse it in a tray filled with deionized water/tap water (see Fig. 13) for 5 min.)
- 5) Visually check the outer surface of the Attachment for cleanness. If necessary, use magnifying glass for visually check. If there is still soil visible, repeat all above steps.

Manual disinfection:

A) EUP-C514 probe

- 1) Prepare the disinfectant solution in a tank with cold water (please follow the instructions of the disinfectant manufacturer regarding application, concentration, microbiological efficiency, service life and contact time).
- 2) Confirm the concentration of the disinfectant before immersing the probe. Although Cidex® OPA does not need to be diluted, it is recommended to use test strips to verify the concentration. The test strips can indicate whether or not the concentration is above the Minimum Effective Concentration (MEC). Please also note the expiration date of the test stripes. Temperature of disinfectant solution should be minimum 20 °C. The minimum contact time is 5 minutes. If a different disinfectant is used, follow the manufacturer's instructions. Please also consider the material compatibility for the medical device.

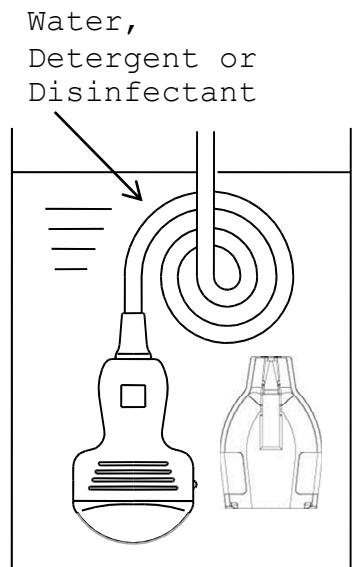


Fig. 13 Immersion of the probe

- 3) Immerse the immersible part of the probe into the disinfectant (see Fig. 13). Set a clock to insure the recommended contact time which is 5 minutes.
- 4) Rinse the immersible part of the probe with deionized water for 1 minute. (alternatively: immerse the immersible part of the probe in a tray filled with deionized water (see Fig.18) for 5 min.)
- 5) Visually check the outer surface of the probe for leavings of the disinfectant. If necessary, repeat the rinsing.

B) Magnetic Sensor Attachment

- 1) Prepare the disinfectant solution as stated in the procedure for the probe.
- 2) Immerse the Attachment into the disinfectant (see Fig. 13). Set a clock to insure the recommended contact time which is 5 minutes.
- 3) Rinse the Attachment with deionized water for 1 minute. (alternatively: immerse it in a tray filled with deionized water (see Fig.18) for 5 min.)
- 4) Visually check the outer surface of the Attachment for leavings of the disinfectant. If necessary, repeat the rinsing.

5.4. Drying

Drying

- 1) Wipe the probe with a single-use, fluff-free wipe or towel to remove moisture from the surface of the probe.
- 2) Dry the probe naturally in an ambient temperature between 15-30°C for a minimum of 4 hours. Alternatively the equipment can be dried using a drying heater at a temperature of less than 55 °C.

5.5. Inspection

Inspect the equipment for any damage such as crack, scratch or deformation. Do not use it if any damage is found.

5.6. Packaging

Packaging

Pack the probe in a sterile barrier such as Polypropylene fleece or transparent package made from Polyethylene film and Tyvek®, and then place it into a tray. The tray should be also covered with a sterile barrier.

Additionally the probe can be placed on plastic mesh wires supplied for plasma sterilization and then packed as mentioned above.

The probe can be packed in a simple or double packing.

Please note that the size of a sterile barrier should be large enough to be able to pack the equipment leaving sufficient space to seal it completely.

A sterile barrier should be sealed by an appropriate sealing machine and it is important to confirm that the package is sealed completely. If the sealing is not complete, pack and reseal again.

5.7. Sterilization

Sterilization

The probe and accessory can be sterilized using either ethylen oxide gas (EtO) sterilization or plasma sterilization (see table in the next page).

Follow the manufacturer's instructions of the sterilizer regarding usage, temperature and sterilization-time.

The sterilization method and operating conditions are as follows.

Sterilization Method	Condition
Plasma Sterilization: STERRAD® 50, 100S or 200 (*)	Short Cycle
Plasma Sterilization: Sterrad® NX or 100NX (*)	Standard cycle
ETO Sterilization	<ul style="list-style-type: none"> ➤ Gas Type: 10% EO/ 90% HCFC ➤ Temperature: 50-55°C ➤ Exposure Time: More than 120 minutes ➤ Pressurization: 162-200kPa Depressurization: 13-8kPa ➤ Relative humidity: 40-90% ➤ Aeration is minimum 12 hours

* STERRAD® systems are manufactured by "Johnson & Johnson"

! WARNING

- 1) Before performing sterilization, check that the operation data of sterilizer are in conjunction with min. and max. data applicable for the probe and the Attachment.
- 2) Do not sterilize the probe and the Attachment by Steam Autoclaving. If you autoclave them, they suffers serious damage and will be not functional.

The packaging procedure is as follows.

- 1) Put the probe into TYVEK pouch.

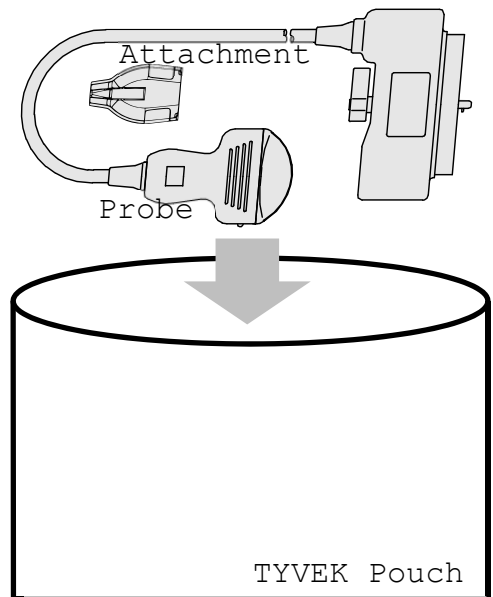


Fig. 14 Packaging in the pouch

- 2) Seal the TYVEK Pouch using a heat sealer. Ensure that the seal is complete.

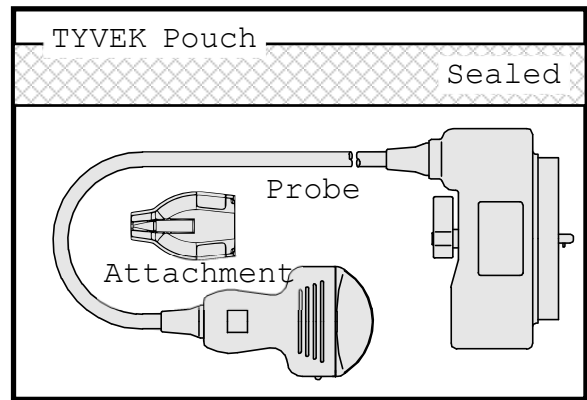


Fig. 15 Sealing

- 3) Put the sealed pouch into a tray or plastic mesh wire for sterilization.



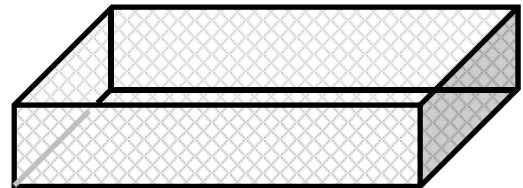


Fig. 16 Packaging in a tray

5.8. Storage

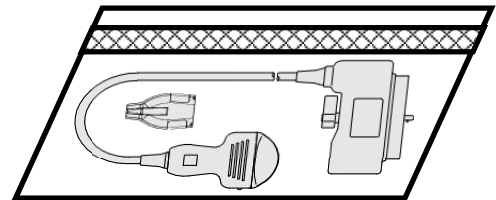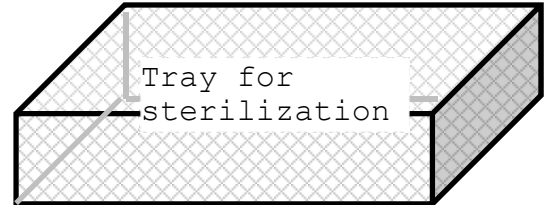

Store the equipment in a cool, dustproof and dark space to avoid high temperature, humidity and direct sunlight. Limitations for the time for sterilized equipment belong to package.

6. Maintenance and Safety Inspection



- 1) After using the probe, the probe should be cleaned and disinfected or sterilized according to “5. Reprocessing Procedure of the probe”, store the probe in a cool and dark space to avoid high temperature, humidity and direct sunlight.
- 2) Visually inspect the surface of the probe head, the housing, the cable and the connector for any crack, scratch or denaturalization. If you find any damage, do not use the probe, and contact a service support immediately.
- 3) After using the Magnetic sensor attachment and the Spacer for EZU-RV2S, the Magnetic sensor attachment and the Spacer for EZU-RV2S should be cleaned and disinfected or sterilized according to “6. Reprocessing Procedure of the Magnetic Sensor Attachment”, store the Magnetic sensor attachment and the Spacer for EZU-RV2S in a cool and dark space to avoid high temperature, humidity and direct sunlight.
- 4) Visually inspect the surface of the Magnetic sensor attachment and the Spacer for EZU-RV2S for any crack, deformation or denaturalization. If you find any damage, do not use them, and contact a service support immediately.

7. Safety Precautions

〈WARNING〉

- Never use the probe if the probe head, housing or cables are cracked or damaged.
- Warning is case of using probe covers which latex is contained to. The latex may cause such allergic reactions as itching, rubor, urticaria, swelling, fever, anhelation, wheezing, and depression of blood pressure, shock and so on. For the patients suspected of latex allergy, do not use the latex-containing medical devices. If you observe any of above mentioned symptoms in your patient during the operation, stop the use of the latex-containing medical devices immediately and take an appropriate treatment to the patient.

〈CAUTION〉

- Keep the acoustic power low and minimize the ultrasound exposure time for the examination of an early pregnancy.
- Do not expose the connector to water or other liquids. The connector is not waterproof.
- Do not hit or drop the probe. The probe is easily damaged by mechanical shock.
- Do not use detergents and disinfectants other than listed in “9.2 Suppliers list”.
- Use a sterile probe cover to avoid staining or damaging the acoustic lens.
- Clean and sterilize the probe, the Magnetic sensor attachment and the Spacer for EZU-RV2S before the first use as it is not sterilized in the factory.
- Use only the soft cloth or tissue to clean the acoustic lens.
- A biopsy should be performed only by a well-trained physician.
- Do not attach unapproved devices to the probe.

8. Specification

8.1. Probe

Type:	EUP-C514 Convex Array probe
Center frequency:	3.5MHz
Technology:	Convex Array Probe
Dimensions:	See Fig. 17
Weight:	Approx. 0.9kg (incl. cable and connector)
Scanning angle:	90°
Probe materials:	Bio-compatible allergy free components
Acoustic output:	According to IEC60601-2-37 (See Main Unit manual.)
Applicable system:	Depending on production and upgrade status. For detailed information contact a service support.
Classification:	MDD classification IIa.
Cleaning:	Applicable detergents are listed in the suppliers list
Disinfection:	Applicable disinfectants are listed in the suppliers list
Sterilization:	ETO gas sterilization or Plasma sterilization
Operating conditions:	
Ambient temperature;	25 to 35°C
Contact surface temperature max. 42°C (temperature of examinee);	
Relative humidity;	30 to 85%
Storage conditions:	
Temperature;	-10 to +55°C
Relative humidity;	10 to 95% (subject to no condensation)

8.2. Suppliers List

The products listed below are seriously tested and approved for use with the convex array probe EUP-C514.

Product name	manufacturer	purpose
ALKACIDE	ALKAPHARM	Disinfectant
ALKAZYME	ALKAPHARM	Cleaner
ANIOXYDE 1000	ANIOS	Disinfectant
CIDEX	Johnson & Johnson	Disinfectant
CIDEX OPA	Johnson & Johnson	Disinfectant
CIDEX plus	Johnson & Johnson	Disinfectant
Cidezyme	Johnson & Johnson	Enzymatic detergent
Incidin Liquid	Henkel Hygiene GmbH	Disinfectant
Incidur Spray	Henkel Hygiene GmbH	Disinfectant
Meliseptol HBV-Tücher	Braun	Disinfectant
STERANIOS 2%	ANIOS	Disinfectant
Sterile protection Product	International Medical	Covers
Transducer covers	CIVCO Medical	Covers
Tristel 1 Day	Tristel Company	Disinfectant
Tristel Multi-Shot	Tristel Company	Disinfectant
Virkon S	ANTEC	Disinfectant

Please contact your local distributor for a current version of the "Disinfectant/Sterilization Method Compatibility for Ultrasound Probe and Accessory List

9. Disposal of the probe

Please contact us or the distributor for disposal of the probe.

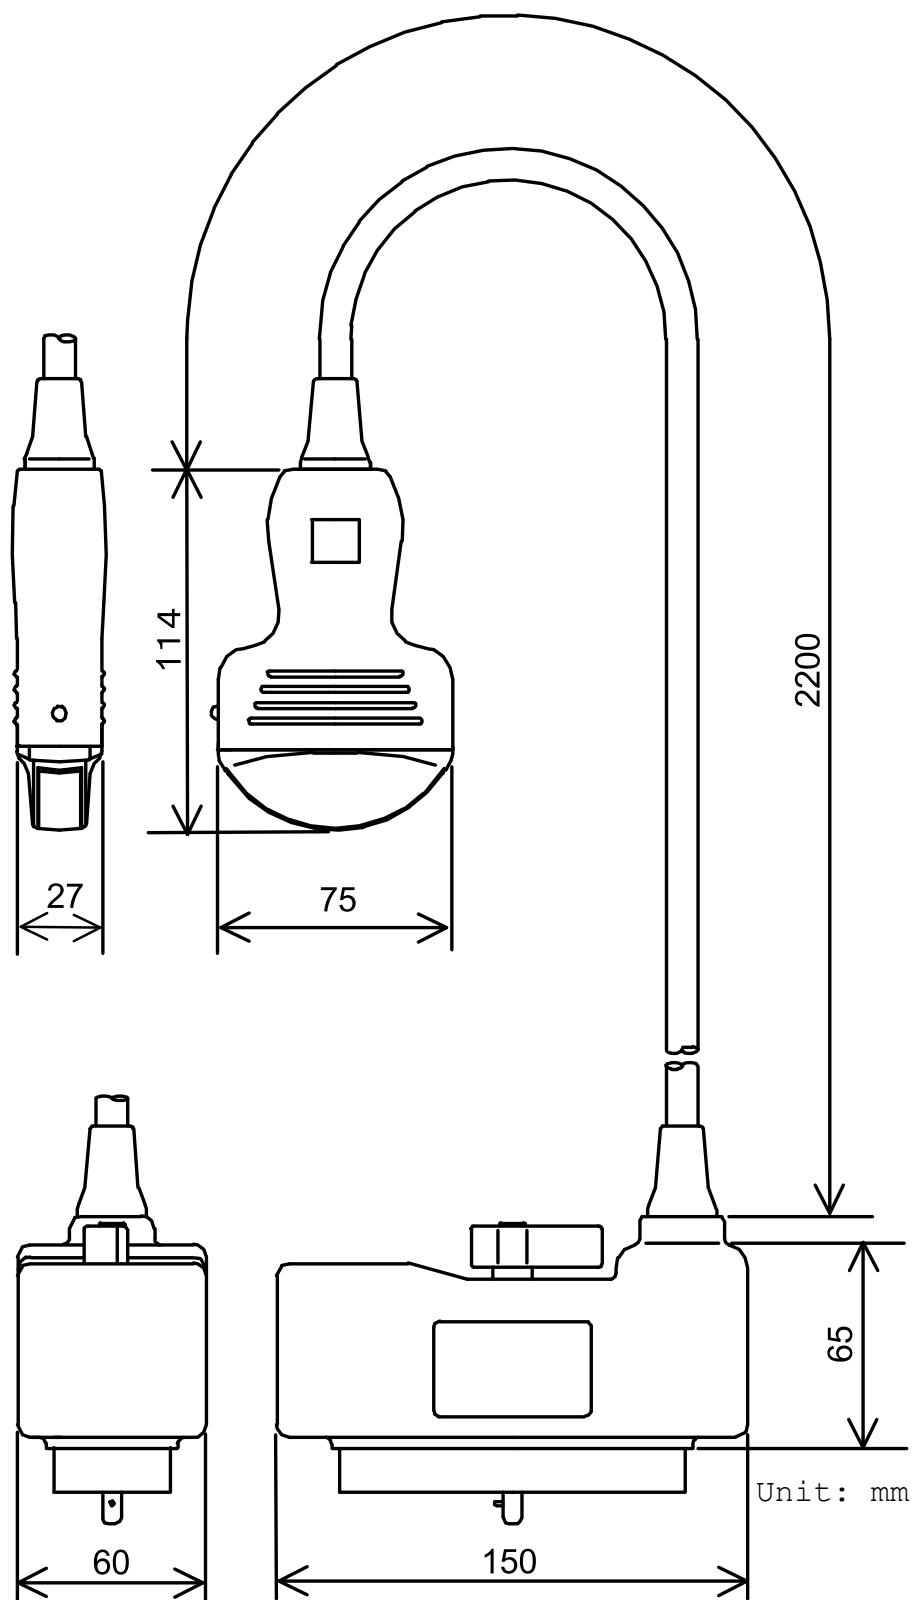


Fig. 17 Dimensions